

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
 Data File : FG005337.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2019 22:34
 Operator : DD\AJ
 Sample : K3605-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 00:37:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	1950470	14.799 ug/ml
Target Compounds			
4) N-TETRADECANE	8.273	13865	0.092 ug/ml
8) N-DOCOSANE	13.876	18796	0.125 ug/ml
10) N-TETRACOSANE	14.977	83471	0.561 ug/ml
11) N-HEXACOSANE	16.006	104279	0.716 ug/ml
12) N-OCTACOSANE	16.957	100352	0.706 ug/ml
13) N-TRIACONTANE	17.847	123278	0.881 ug/ml
14) N-DOTRIACONTANE	18.681	117149	0.871 ug/ml
15) N-TETRATRIACONTANE	19.471	32321	0.252 ug/ml
16) N-HEXATRIACONTANE	20.215	35435	0.297 ug/ml
17) N-OCTATRIACONTANE	20.977	70067	0.661 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
Data File : FG005337.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 22:34
Operator : DD\AJ
Sample : K3605-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:37:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

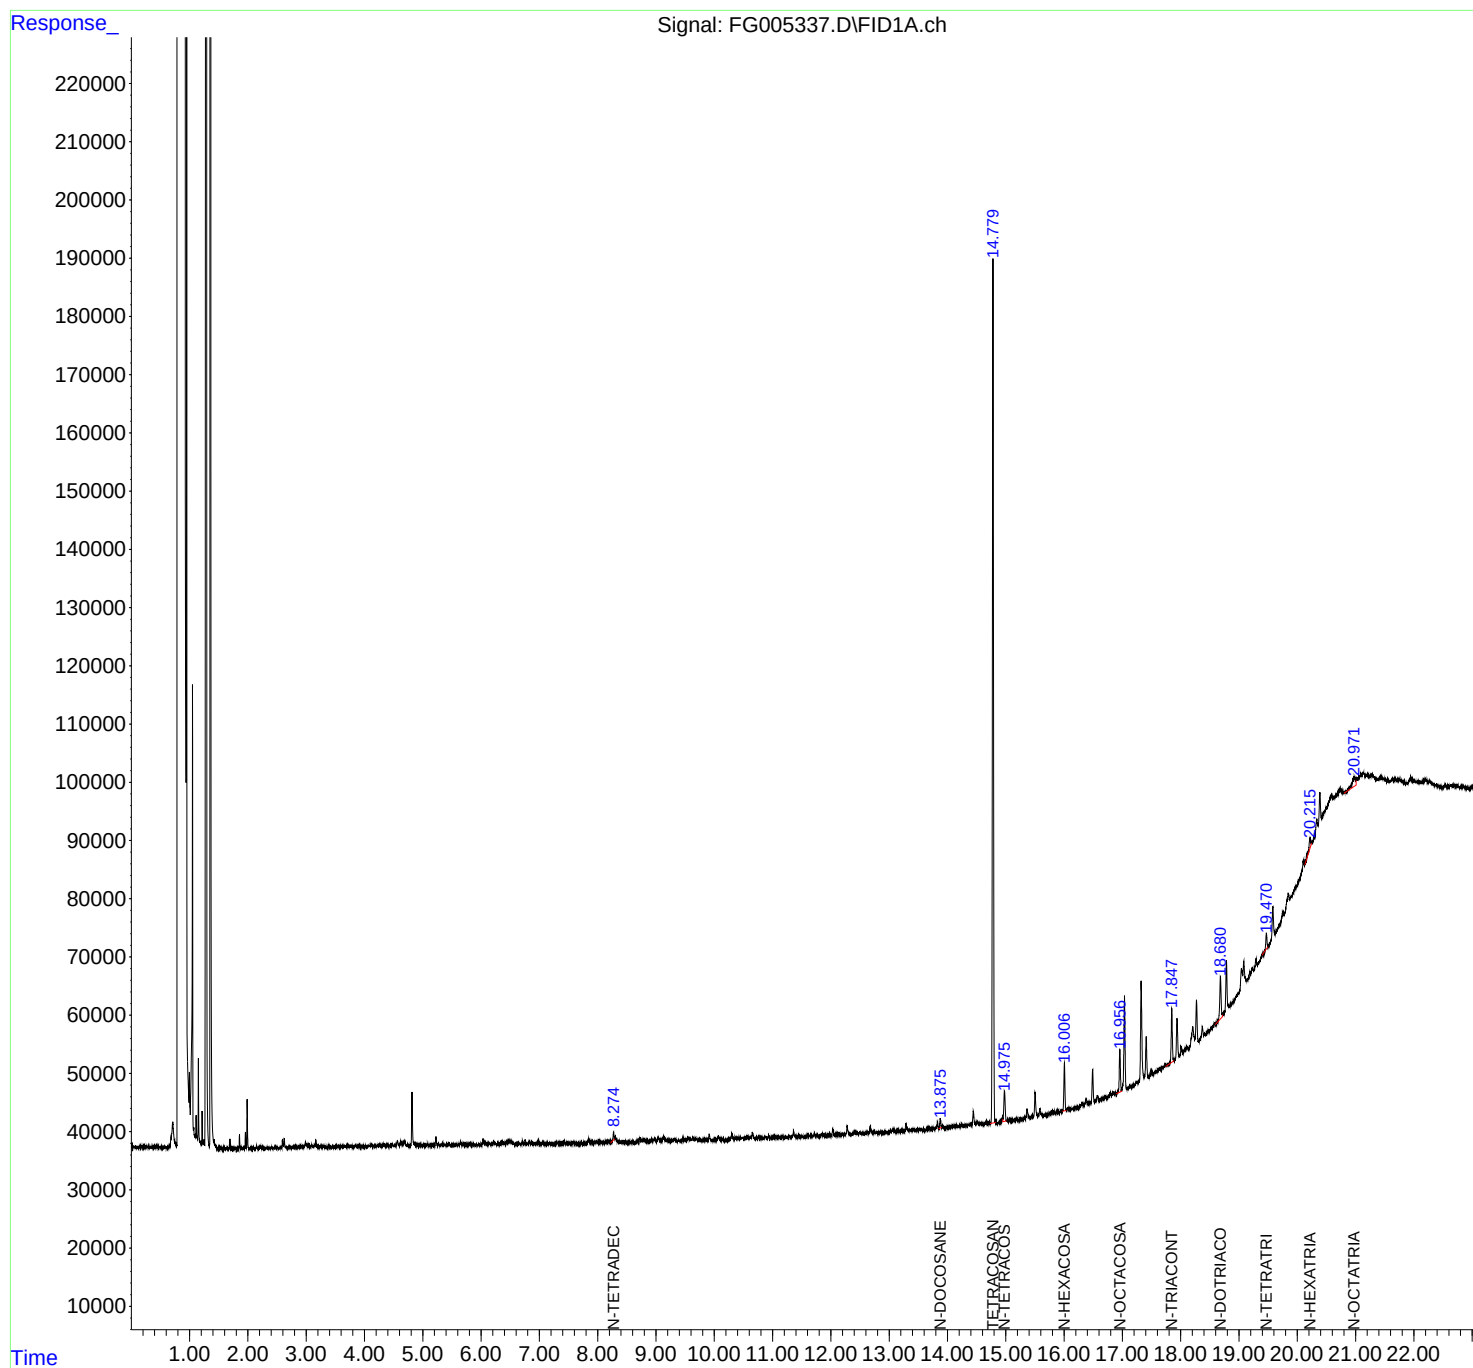


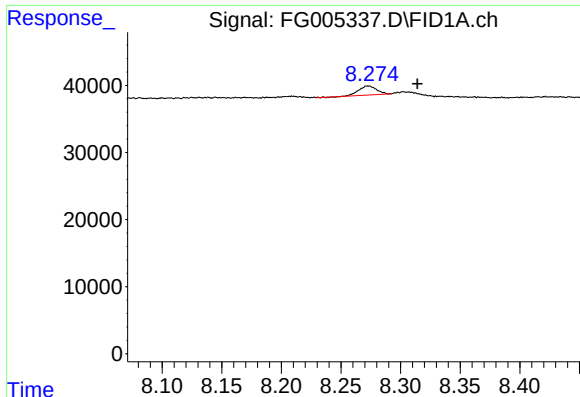

#4 N-TETRADECANE


R.T.: 8.273 min
Delta R.T.: -0.041 min
Response: 13865
Conc: 0.09 ug/ml

Instrument :
FID_G
ClientSampleId :

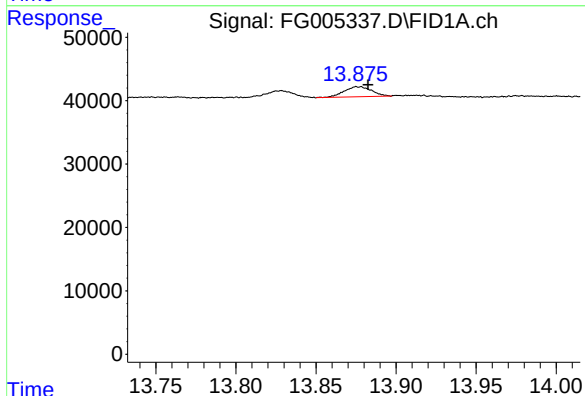


#8 N-DOCOSANE

R.T.: 13.876 min
Delta R.T.: -0.006 min
Response: 18796
Conc: 0.12 ug/ml

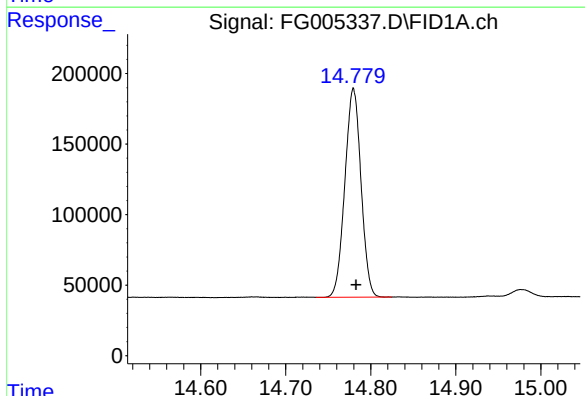


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: -0.003 min
Response: 1950470
Conc: 14.80 ug/ml

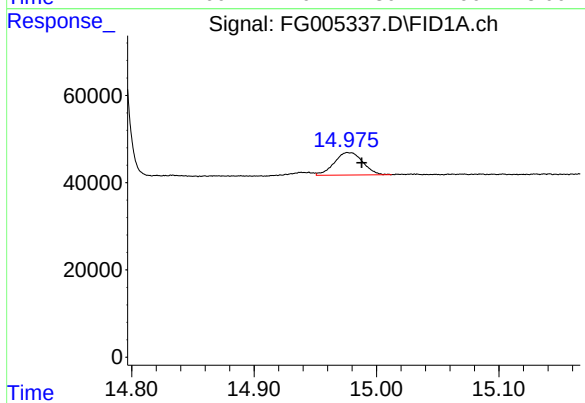

#10 N-TETRACOSANE


R.T.: 14.977 min
Delta R.T.: -0.011 min
Response: 83471
Conc: 0.56 ug/ml

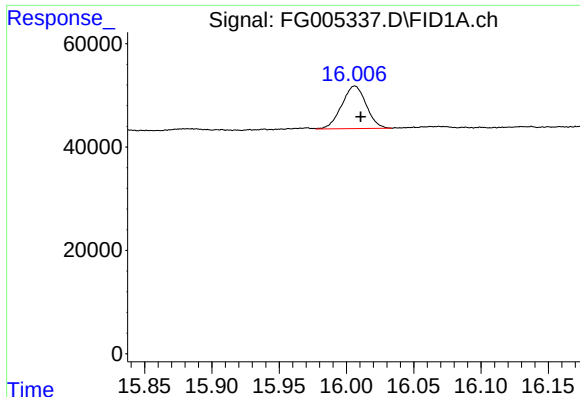

#11 N-HEXACOSANE


R.T.: 16.006 min
Delta R.T.: -0.004 min
Response: 104279
Conc: 0.72 ug/ml

Instrument :
FID_G
ClientSampleId :

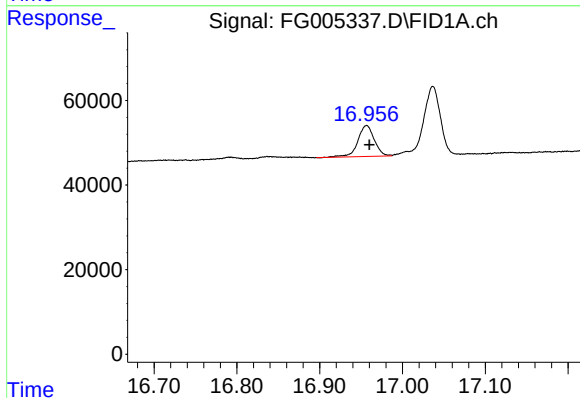


#12 N-OCTACOSANE

R.T.: 16.957 min
Delta R.T.: -0.003 min
Response: 100352
Conc: 0.71 ug/ml

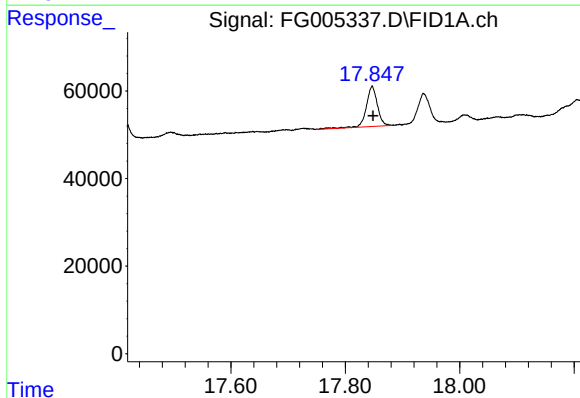


#13 N-TRIACONTANE

R.T.: 17.847 min
Delta R.T.: -0.001 min
Response: 123278
Conc: 0.88 ug/ml

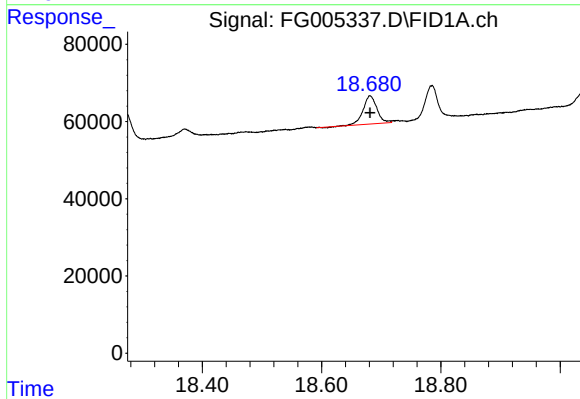

#14 N-DOTRIACONTANE


R.T.: 18.681 min
Delta R.T.: 0.000 min
Response: 117149
Conc: 0.87 ug/ml

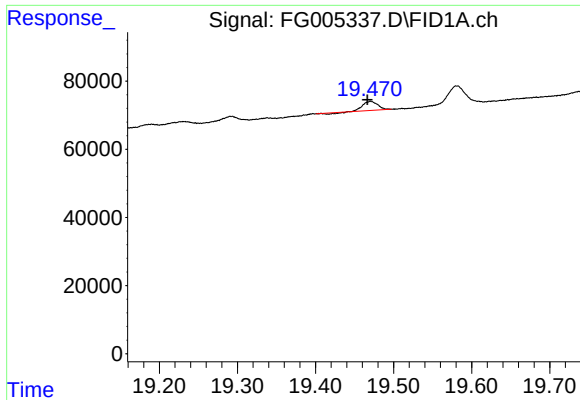

#15 N-TETRATRIACONTANE


R.T.: 19.471 min
Delta R.T.: 0.004 min
Response: 32321
Conc: 0.25 ug/ml

Instrument :
FID_G
ClientSampleId :

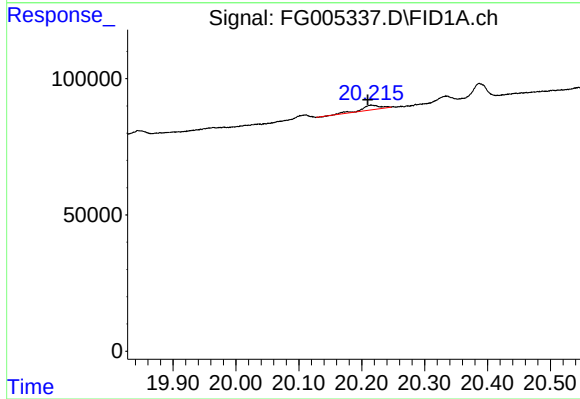

#16 N-HEXATRIACONTANE

R.T.: 20.215 min
Delta R.T.: 0.006 min
Response: 35435
Conc: 0.30 ug/ml

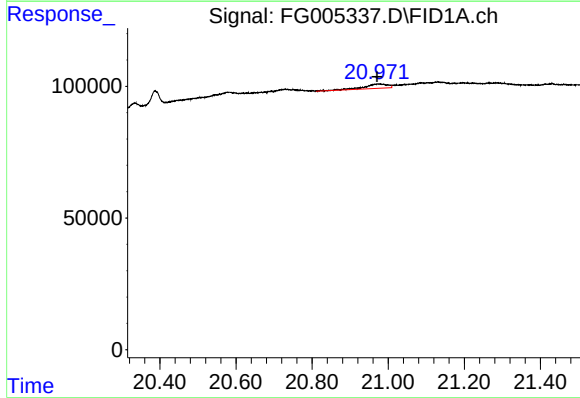

#17 N-OCTATRIACONTANE

R.T.: 20.977 min
Delta R.T.: 0.005 min
Response: 70067
Conc: 0.66 ug/ml