

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
 Data File : FG005338.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2019 23:04
 Operator : DD\AJ
 Sample : PB121096BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 00:37:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	1782627	13.525 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.973	55229	0.371 ug/ml
12) N-OCTACOSANE	16.958	25720	0.181 ug/ml
13) N-TRIACONTANE	17.848	42260	0.302 ug/ml
14) N-DOTRIACONTANE	18.682	56902	0.423 ug/ml
15) N-TETRATRIACONTANE	19.469	16817	0.131 ug/ml
18) N-TETRACONTANE	21.949	74298	0.711 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
Data File : FG005338.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 23:04
Operator : DD\AJ
Sample : PB121096BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:37:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

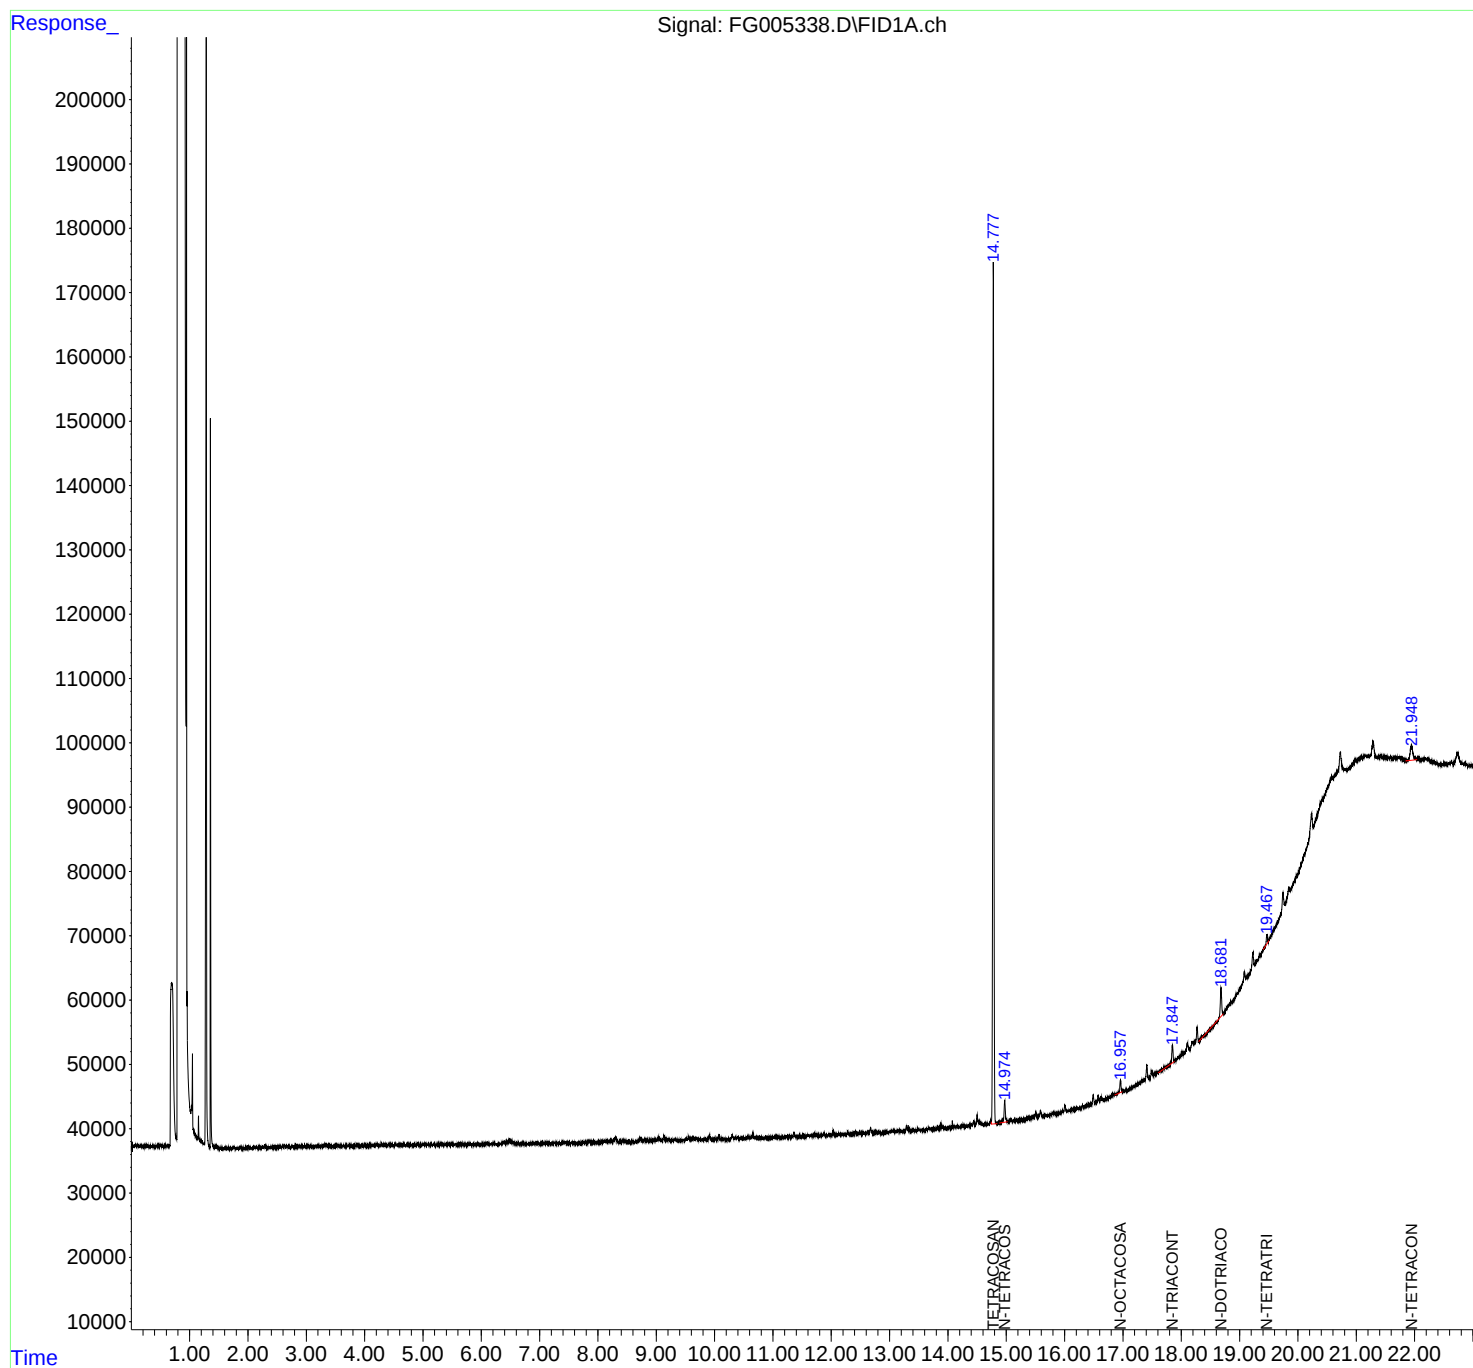


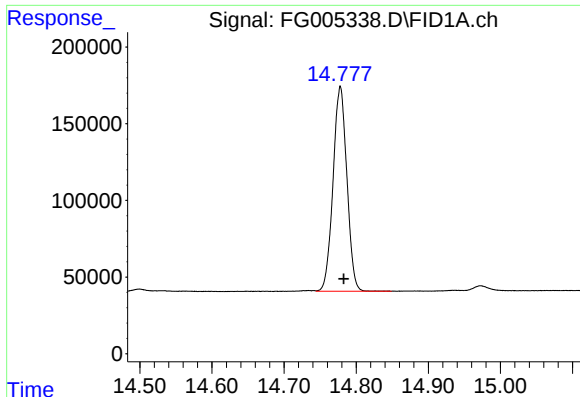

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.778 min
Delta R.T.: -0.005 min
Response: 1782627
Conc: 13.53 ug/ml

Instrument :
FID_G
ClientSampleId :

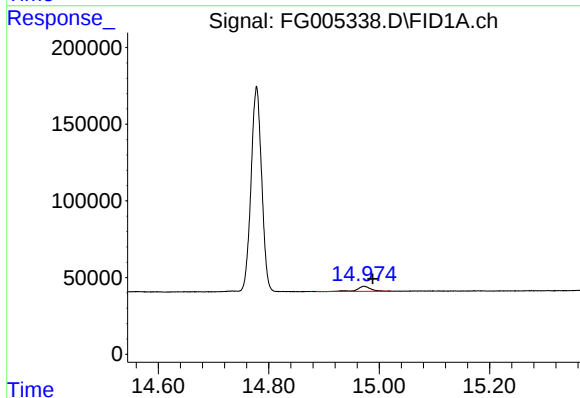


#10 N-TETRACOSANE

R.T.: 14.973 min
Delta R.T.: -0.015 min
Response: 55229
Conc: 0.37 ug/ml

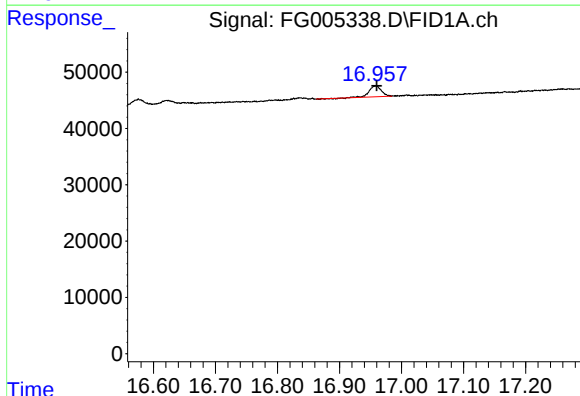


#12 N-OCTACOSANE

R.T.: 16.958 min
Delta R.T.: -0.002 min
Response: 25720
Conc: 0.18 ug/ml

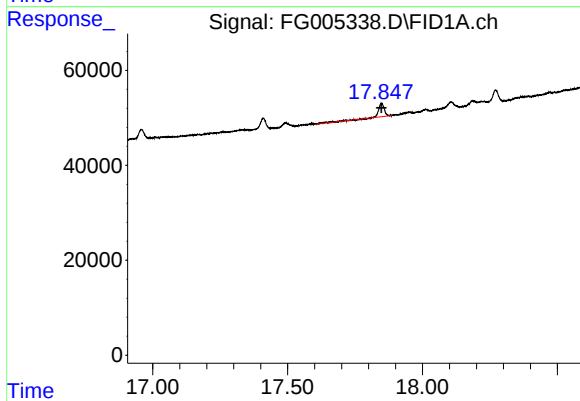

#13 N-TRIACONTANE


R.T.: 17.848 min
Delta R.T.: 0.000 min
Response: 42260
Conc: 0.30 ug/ml

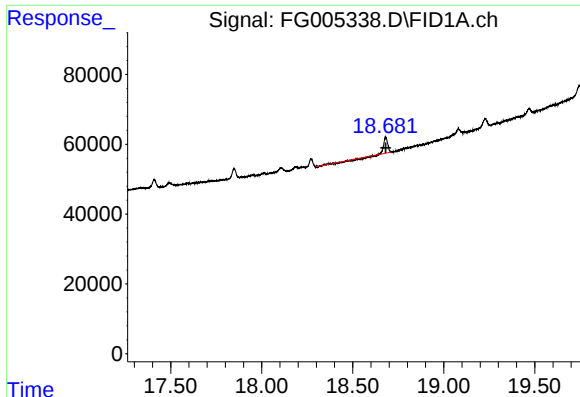

#14 N-DOTRIACONTANE


R.T.: 18.682 min
Delta R.T.: 0.000 min
Response: 56902
Conc: 0.42 ug/ml

Instrument :
FID_G
ClientSampleId :

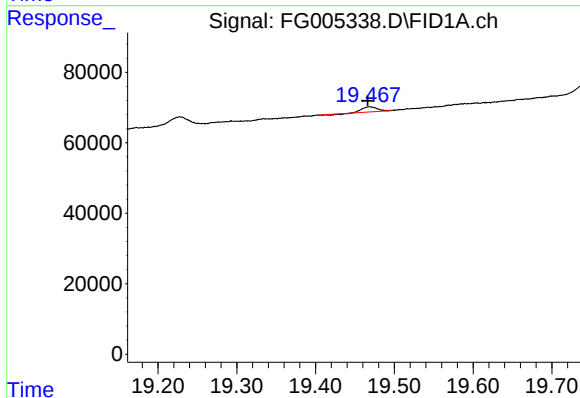

#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: 0.002 min
Response: 16817
Conc: 0.13 ug/ml

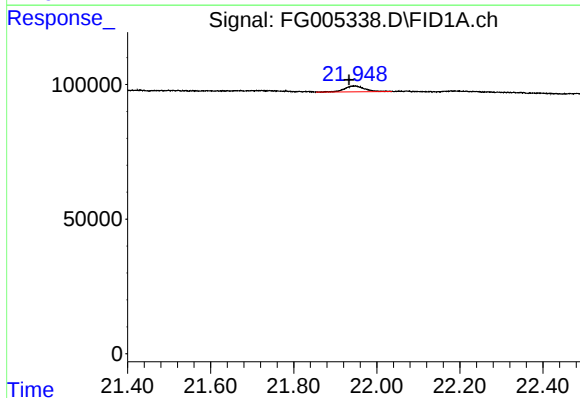

#18 N-TETRACONTANE

R.T.: 21.949 min
Delta R.T.: 0.016 min
Response: 74298
Conc: 0.71 ug/ml