

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
 Data File : FG005341.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jul 2019 00:32
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 07:37:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	2007992	15.235 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.971	47307	0.318 ug/ml
12) N-OCTACOSANE	16.956	35004	0.246 ug/ml
13) N-TRIACONTANE	17.846	62369	0.446 ug/ml
14) N-DOTRIACONTANE	18.680	59367	0.441 ug/ml
15) N-TETRATRIACONTANE	19.467	48903	0.381 ug/ml
17) N-OCTATRIACONTANE	20.975	96273	0.908 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
Data File : FG005341.D
Signal(s) : FID1A.ch
Acq On : 03 Jul 2019 00:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 07:37:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

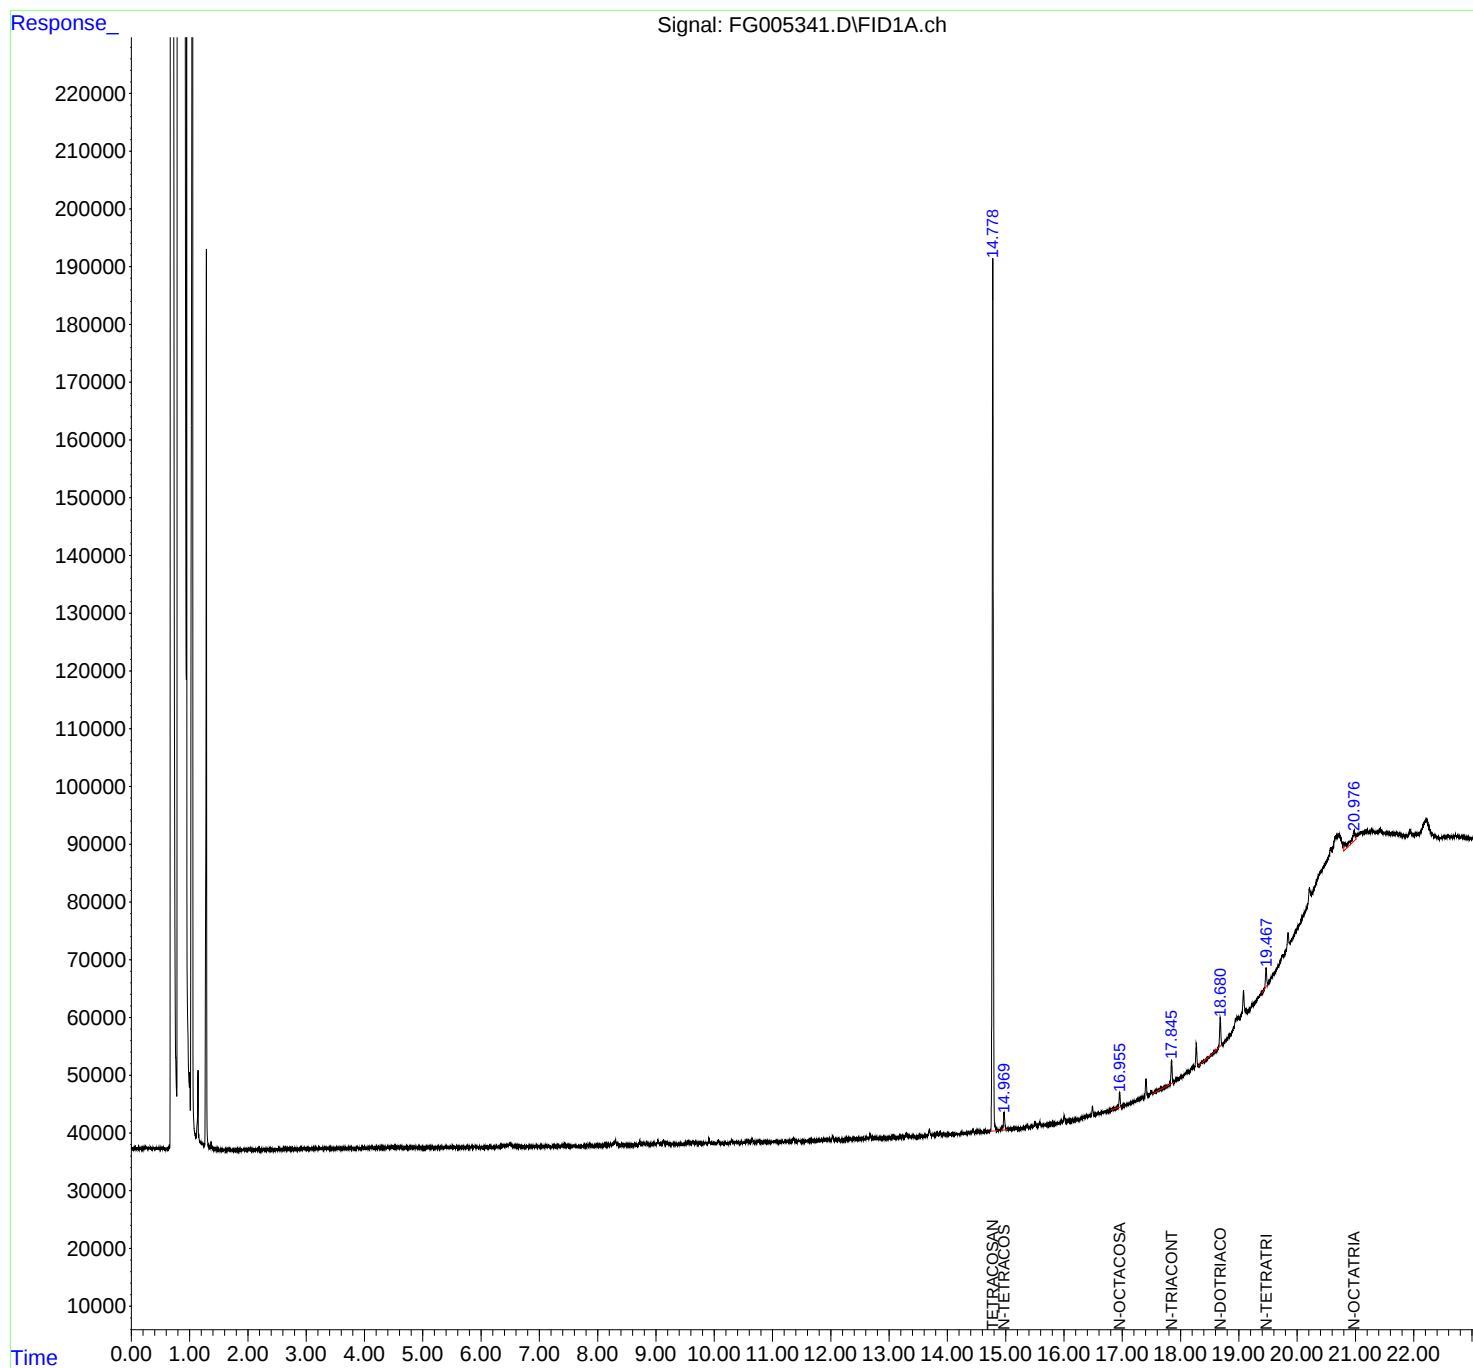


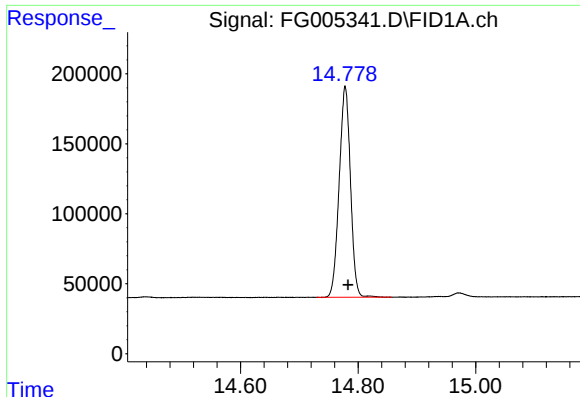

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.778 min
Delta R.T.: -0.005 min
Response: 2007992
Conc: 15.24 ug/ml

Instrument :
FID_G
ClientSampleId :

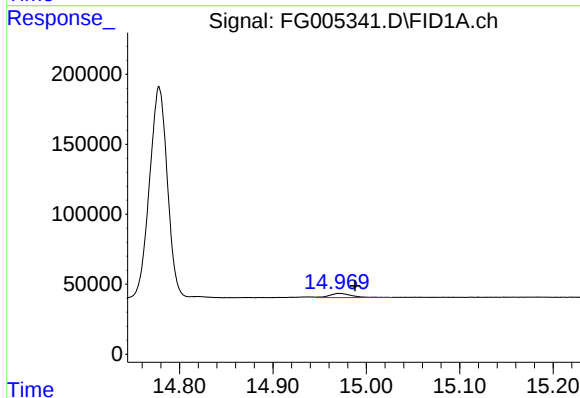


#10 N-TETRACOSANE

R.T.: 14.971 min
Delta R.T.: -0.017 min
Response: 47307
Conc: 0.32 ug/ml

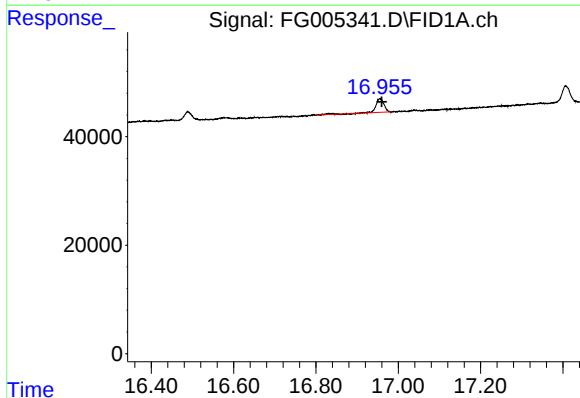


#12 N-OCTACOSANE

R.T.: 16.956 min
Delta R.T.: -0.004 min
Response: 35004
Conc: 0.25 ug/ml

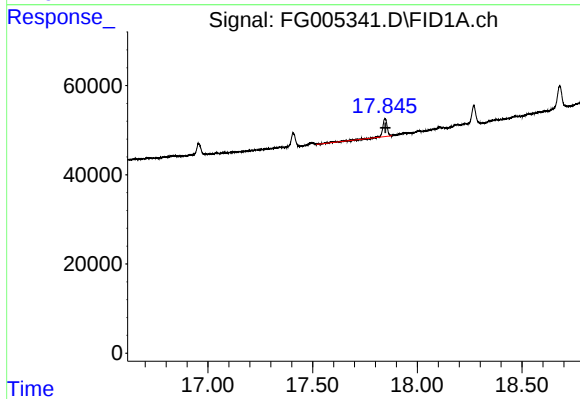

#13 N-TRIACONTANE


R.T.: 17.846 min
Delta R.T.: -0.003 min
Response: 62369
Conc: 0.45 ug/ml

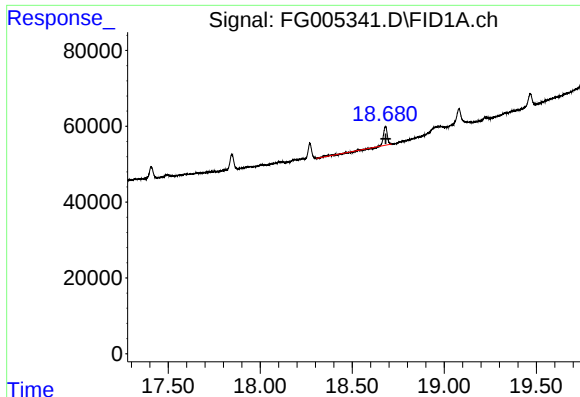

#14 N-DOTRIACONTANE


R.T.: 18.680 min
Delta R.T.: -0.001 min
Response: 59367
Conc: 0.44 ug/ml

Instrument :
FID_G
ClientSampleId :

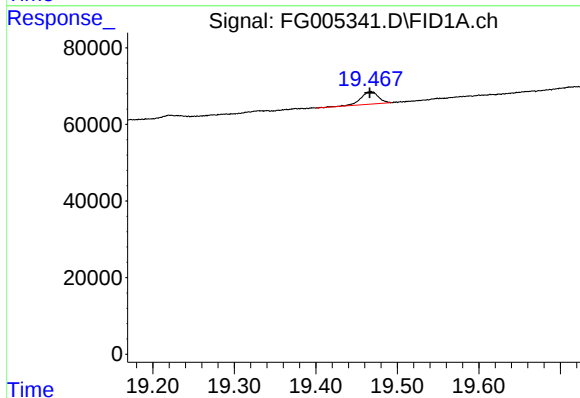

#15 N-TETRATRIACONTANE

R.T.: 19.467 min
Delta R.T.: 0.000 min
Response: 48903
Conc: 0.38 ug/ml

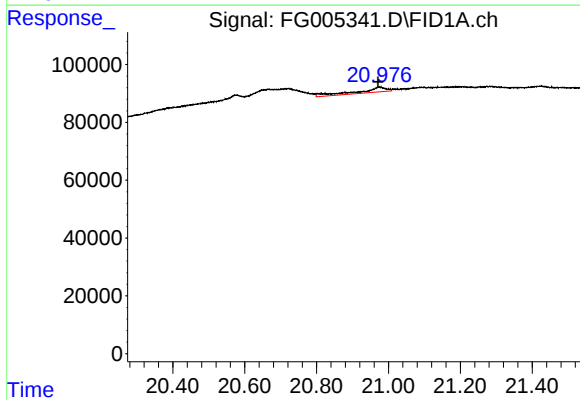

#17 N-OCTATRIACONTANE

R.T.: 20.975 min
Delta R.T.: 0.004 min
Response: 96273
Conc: 0.91 ug/ml