

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070221\
Data File : FG008492.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2021 17:45
Operator : DD\AJ
Sample : M2913-17DL 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 23:12:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.966	419183	2.796 ug/ml
13)	N-TRIACONTANE	17.845	60389	0.429 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070221\
Data File : FG008492.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2021 17:45
Operator : DD\AJ
Sample : M2913-17DL 20X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 23:12:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

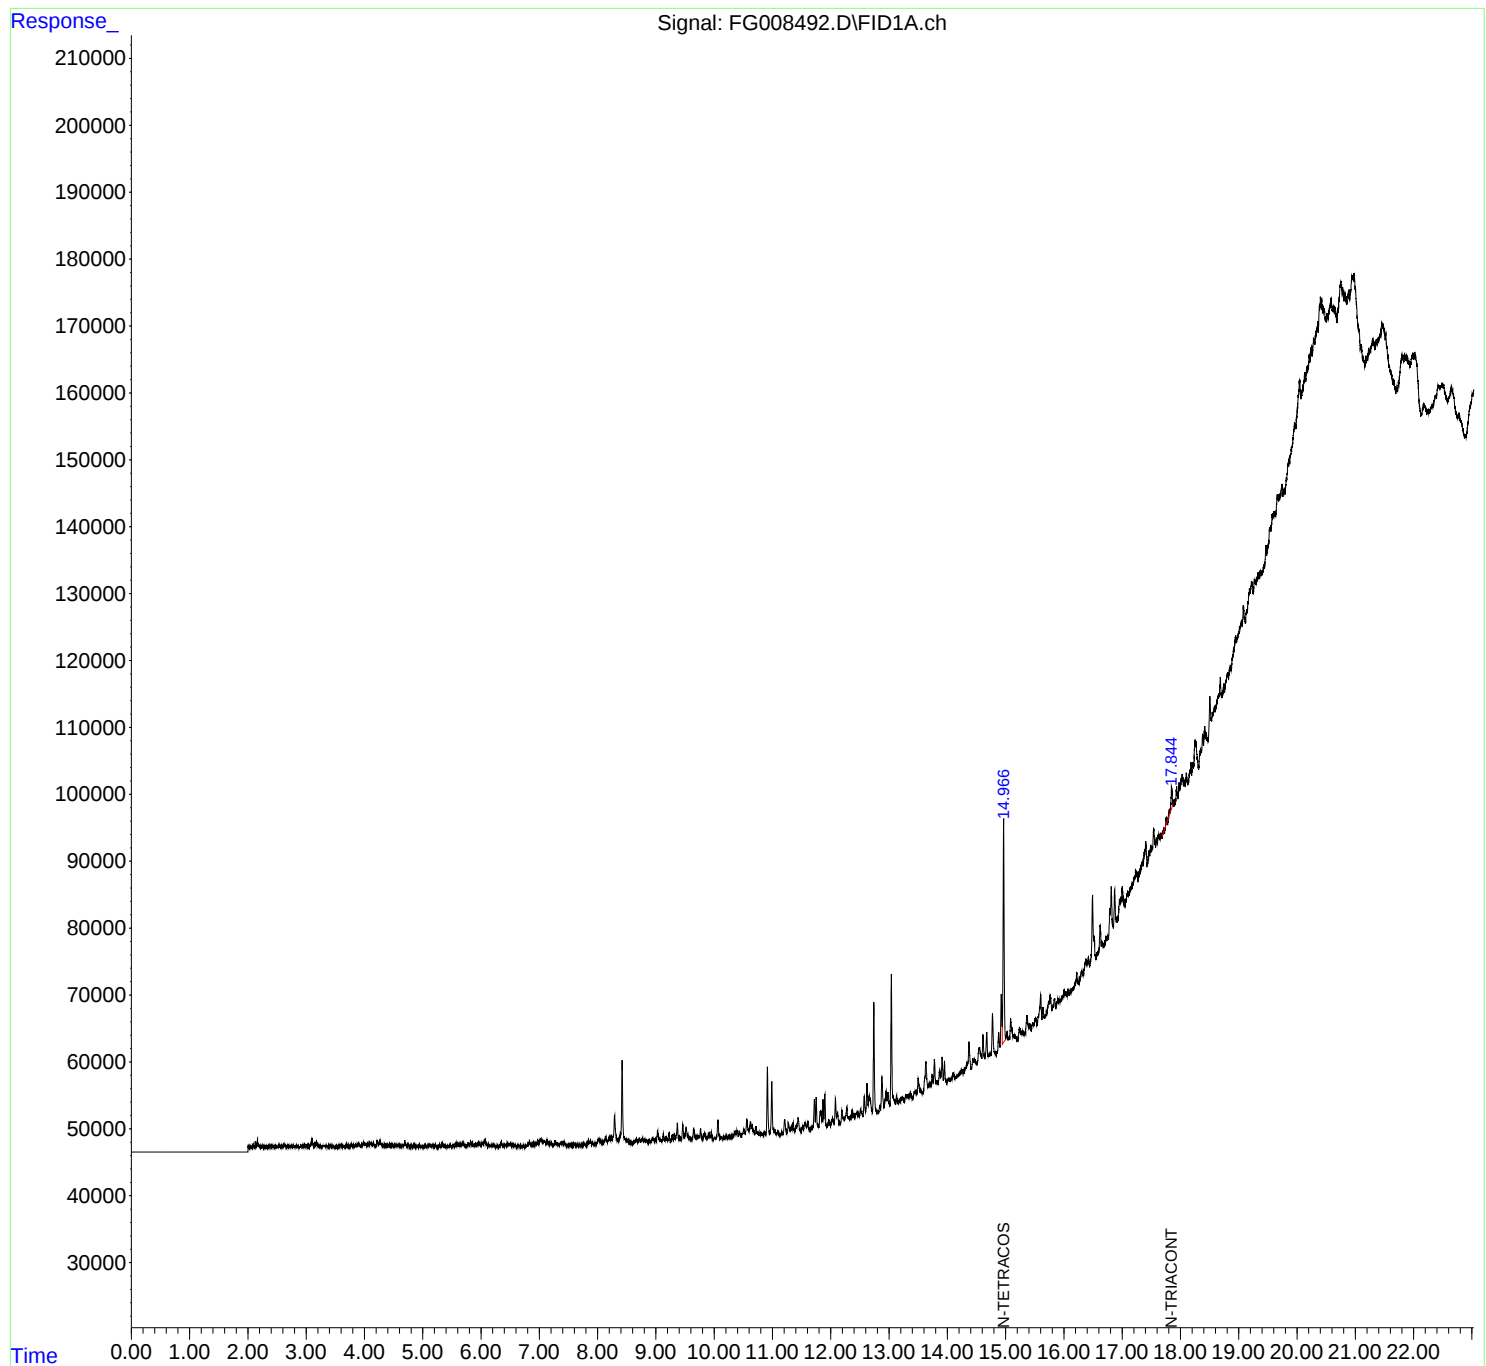


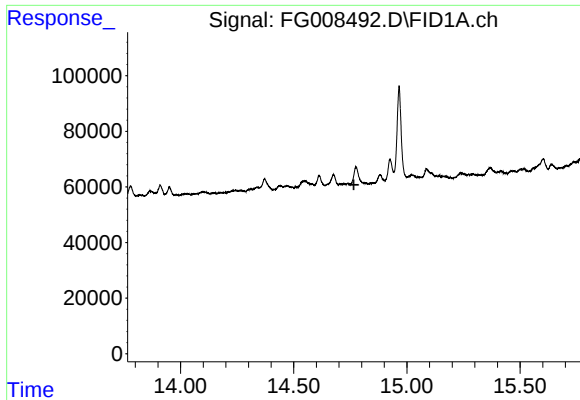

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.766 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

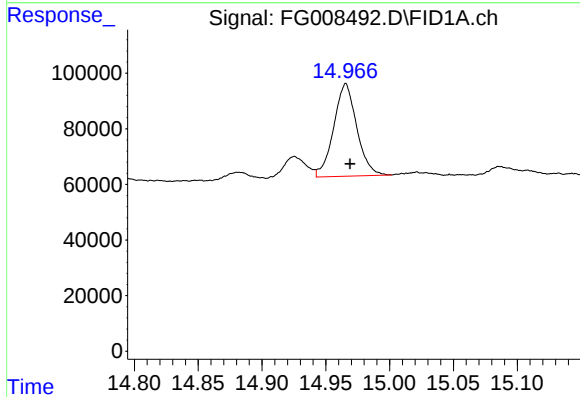

#10 N-TETRACOSANE

R.T.: 14.966 min
Delta R.T.: -0.003 min
Response: 419183
Conc: 2.80 ug/ml

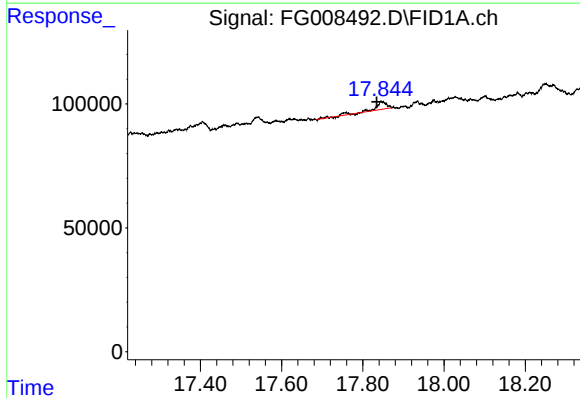

#13 N-TRIACONTANE

R.T.: 17.845 min
Delta R.T.: 0.011 min
Response: 60389
Conc: 0.43 ug/ml