

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070225\
Data File : FG016198.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2025 10:48
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jul 03 01:21:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG061325.M
Quant Title :
QLast Update : Fri Jun 13 12:34:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	18.279	46292	0.358 ug/ml
14)	N-DOTRIACONTANE	19.116	59070	0.476 ug/ml
15)	N-TETRATRIACONTANE	19.904	52822	0.480 ug/ml
16)	N-HEXATRIACONTANE	20.647	79146	0.858 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070225\
Data File : FG016198.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2025 10:48
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jul 03 01:21:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG061325.M
Quant Title :
QLast Update : Fri Jun 13 12:34:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

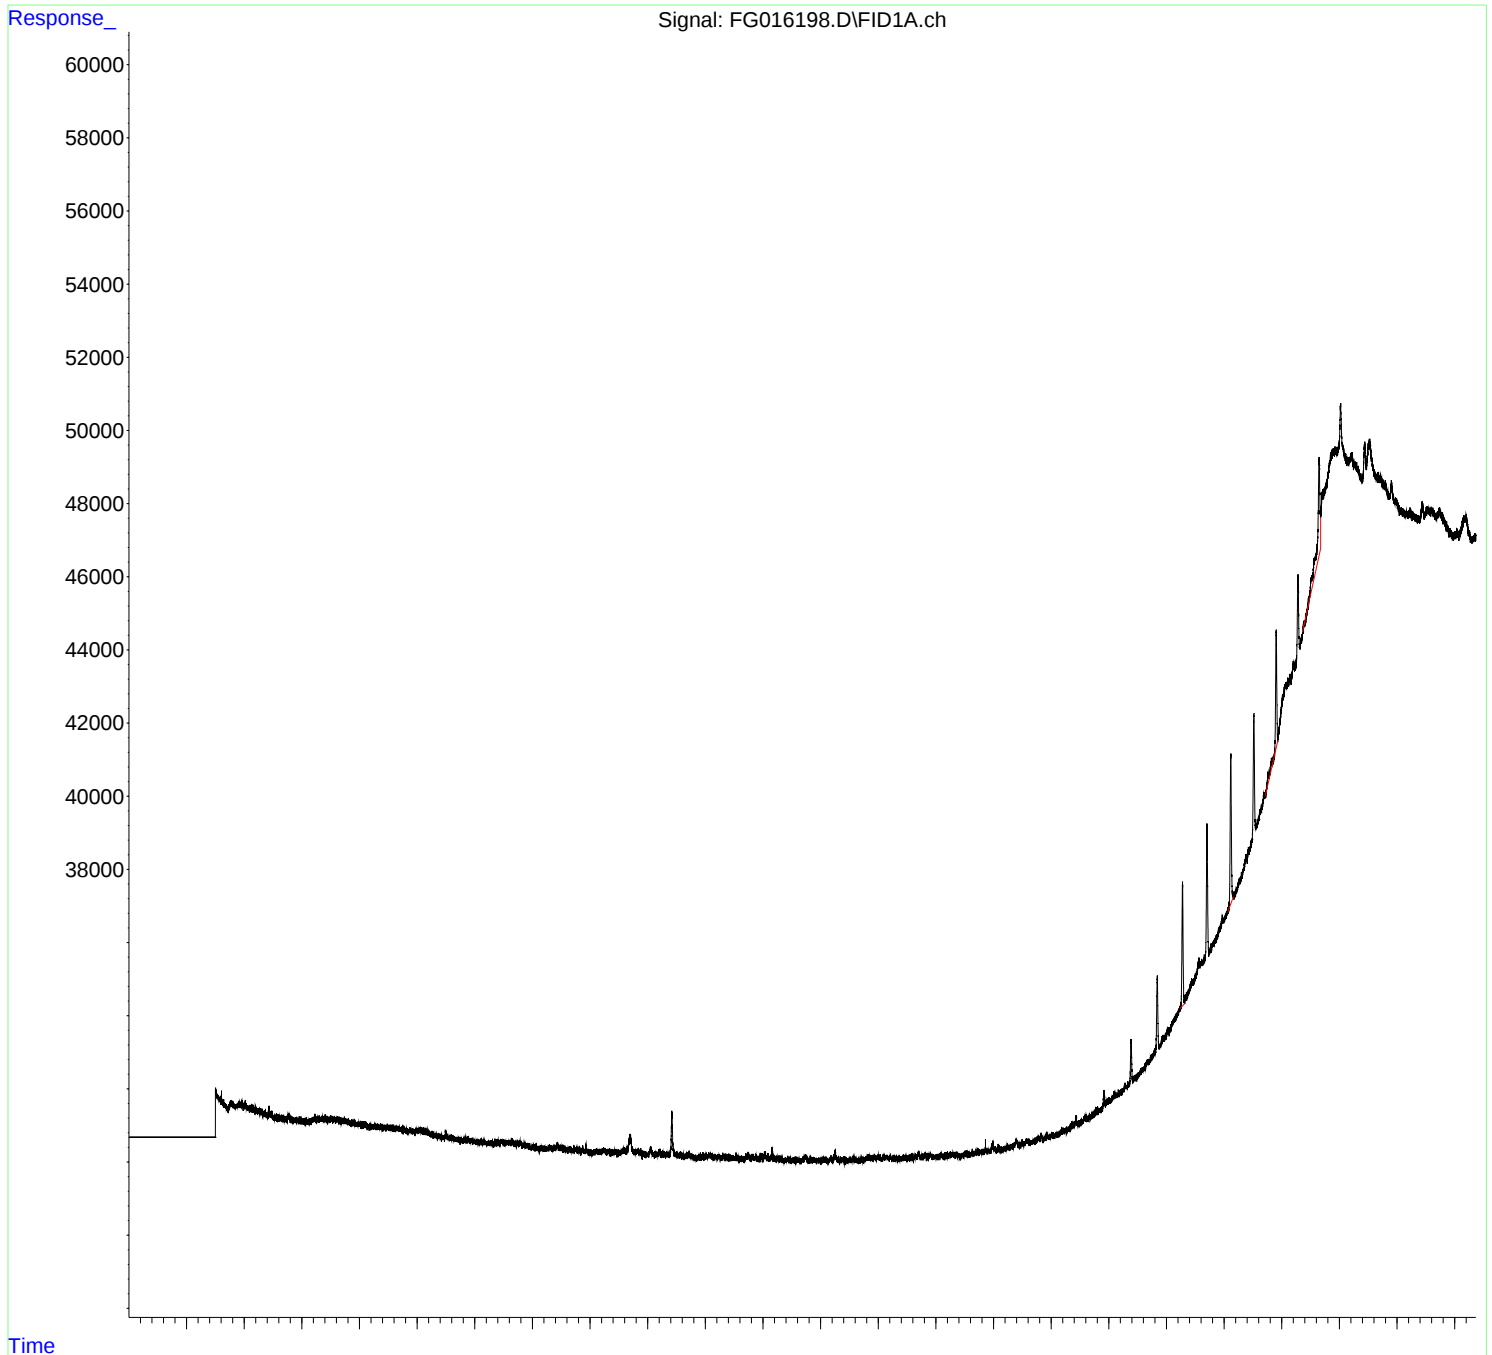


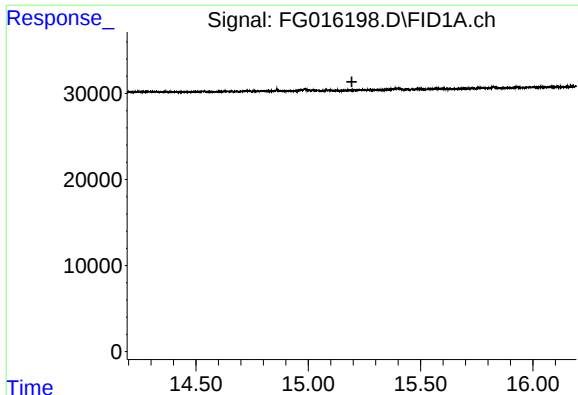

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.194 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
MECL2

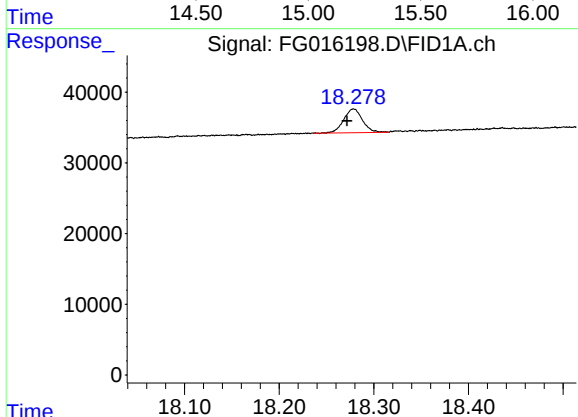


#13 N-TRIACONTANE

R.T.: 18.279 min
Delta R.T.: 0.007 min
Response: 46292
Conc: 0.36 ug/ml

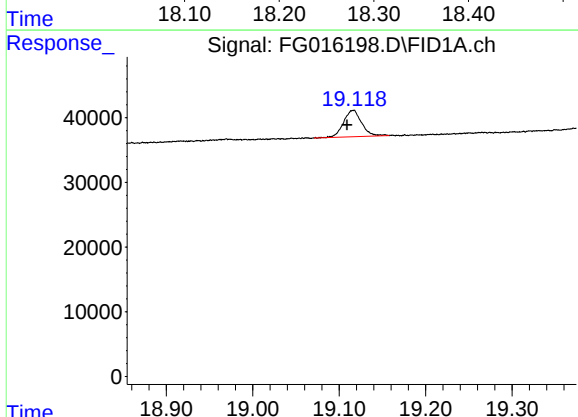


#14 N-DOTRIACONTANE

R.T.: 19.116 min
Delta R.T.: 0.007 min
Response: 59070
Conc: 0.48 ug/ml

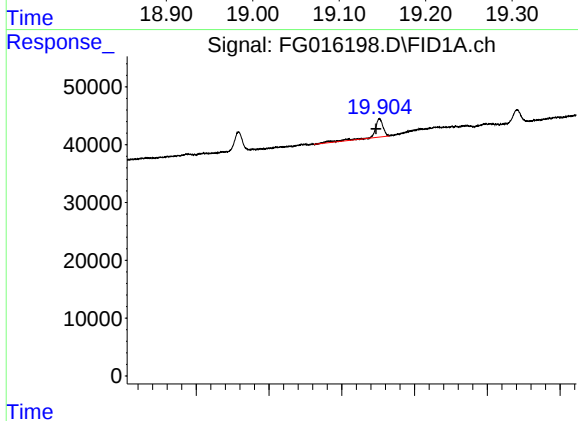

#15 N-TETRATRIACONTANE

R.T.: 19.904 min
Delta R.T.: 0.009 min
Response: 52822
Conc: 0.48 ug/ml

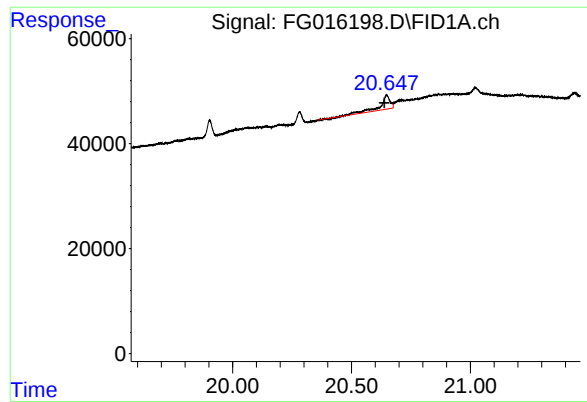

#16 N-HEXATRIACONTANE

R.T.: 20.647 min
Delta R.T.: 0.009 min
Response: 79146
Conc: 0.86 ug/ml

Instrument :

FID_G

ClientSampleId :

MECL2