

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070323AL\
 Data File : FG012321.D
 Signal(s) : FID1A.ch
 Acq On : 03 Jul 2023 08:59
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 04 03:05:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 14:37:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	n-Tetracosane (C24)	14.174	97543	0.733 ug/ml
18) T	n-Dotriacontane (C32)	17.891	95192	0.768 ug/ml
19) T	n-Tetratriacontane (C34)	18.675	68714	0.575 ug/ml
20) T	n-Hexatriacontane (C36)	19.413	9587	0.083 ug/ml
21) T	n-Octatriacontane (C38)	20.166	37170	0.325 ug/ml
22) T	n-Tetracontane (C40)	21.103	23076	0.204 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070323AL\
Data File : FG012321.D
Signal(s) : FID1A.ch
Acq On : 03 Jul 2023 08:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 04 03:05:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 14:37:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

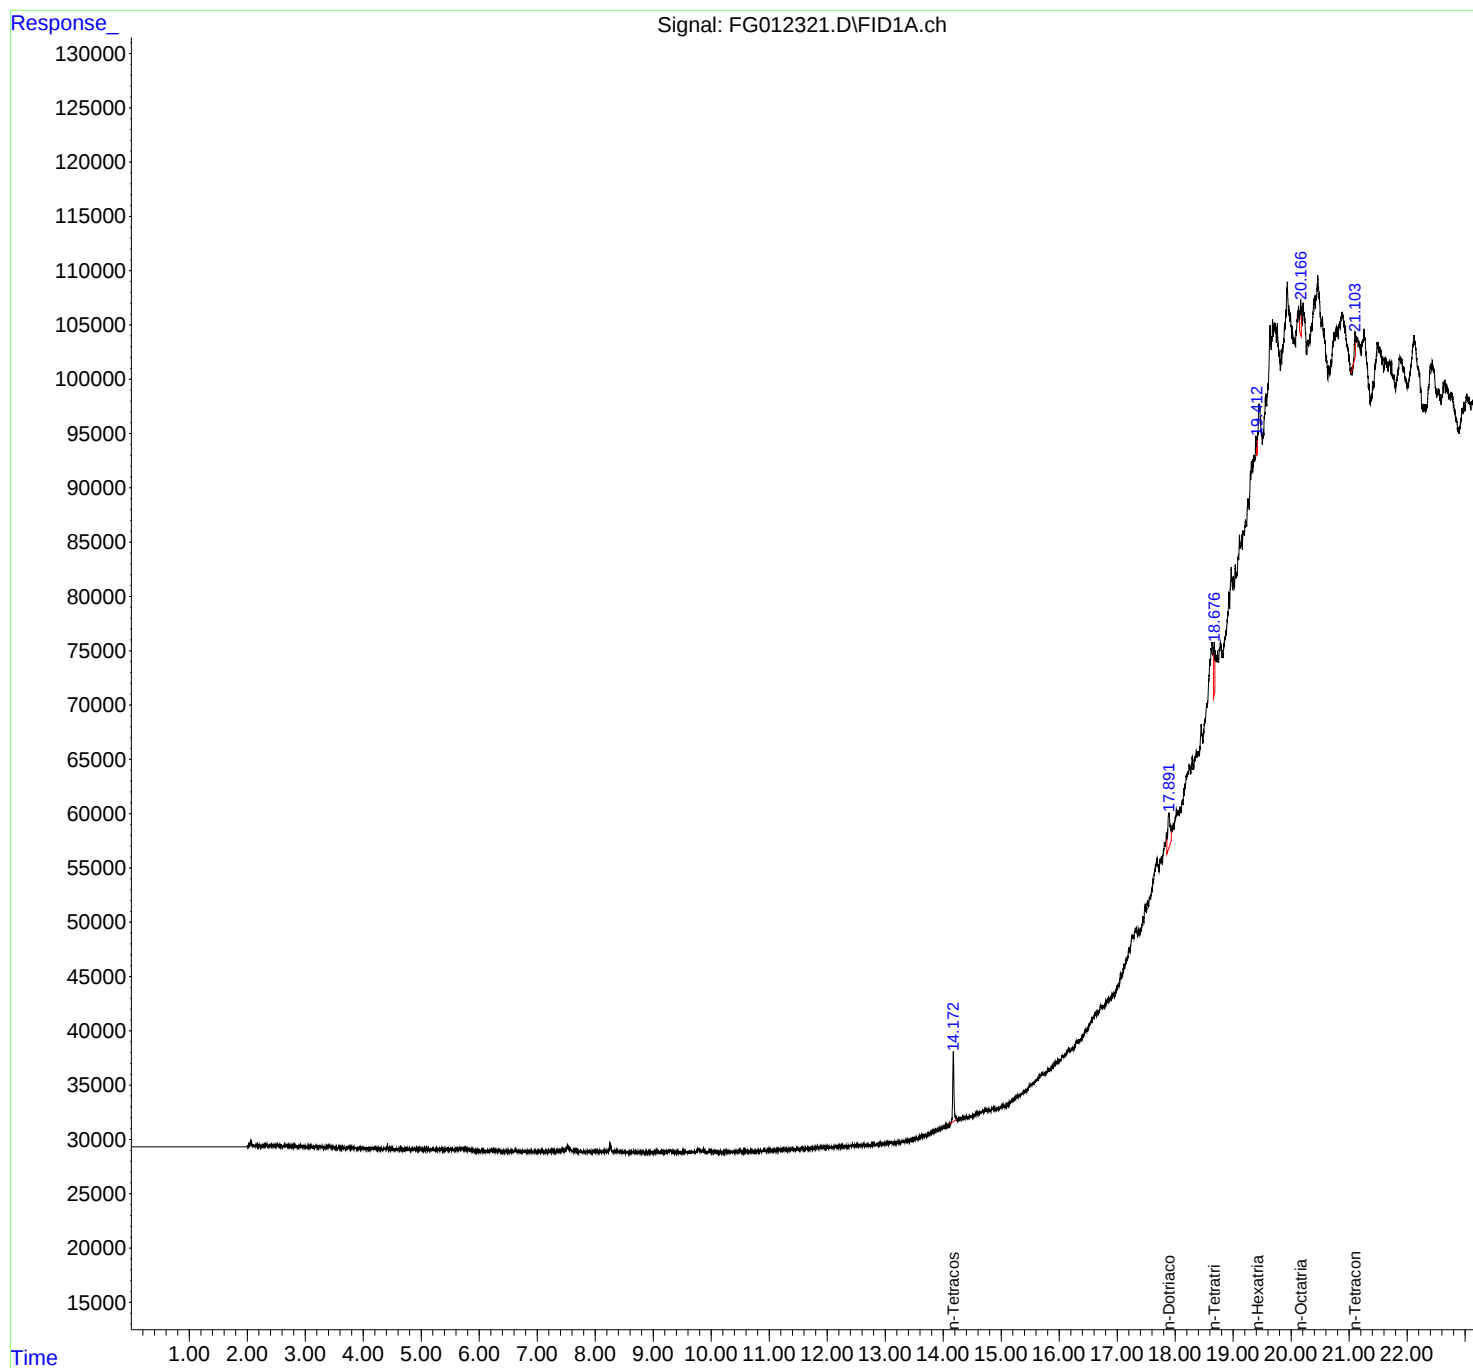


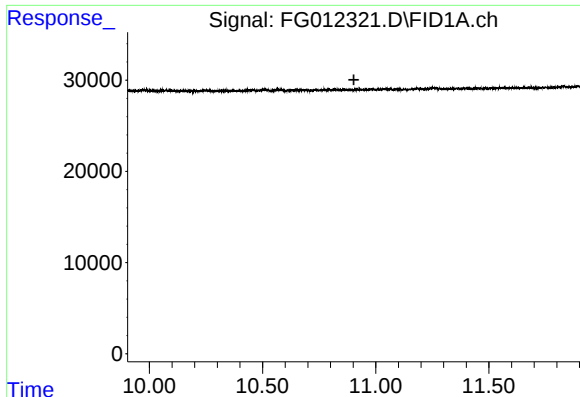

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 10.903 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

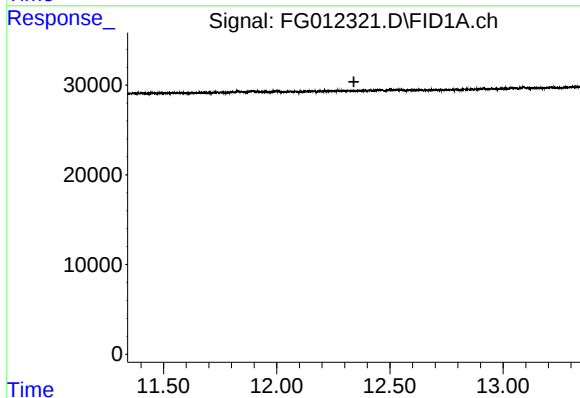


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.341 min
Response: 0
Conc: N.D.

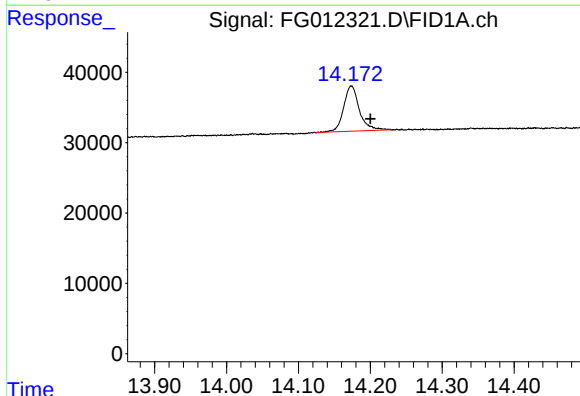


#14 n-Tetracosane (C24)

R.T.: 14.174 min
Delta R.T.: -0.026 min
Response: 97543
Conc: 0.73 ug/ml

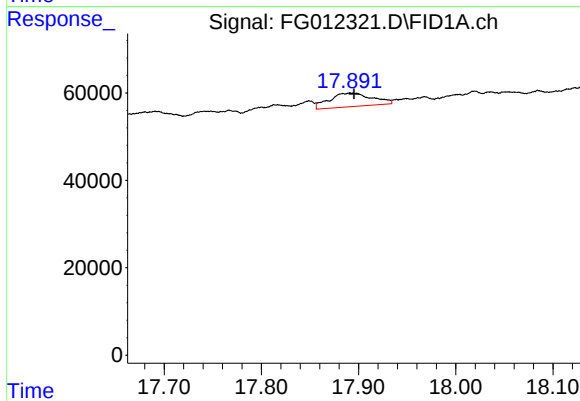

#18 n-Dotriacontane (C32)


R.T.: 17.891 min
Delta R.T.: -0.004 min
Response: 95192
Conc: 0.77 ug/ml

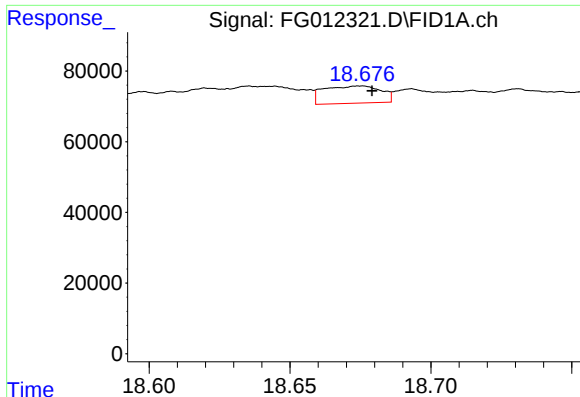

#19 n-Tetratriacontane (C34)


R.T.: 18.675 min
Delta R.T.: -0.004 min
Response: 68714
Conc: 0.57 ug/ml

Instrument :
FID_G
ClientSampleId :

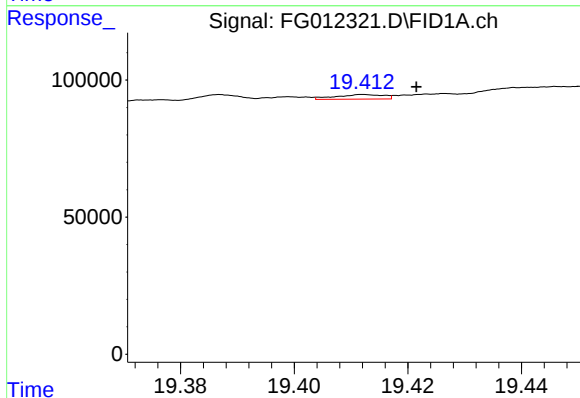


#20 n-Hexatriacontane (C36)

R.T.: 19.413 min
Delta R.T.: -0.009 min
Response: 9587
Conc: 0.08 ug/ml

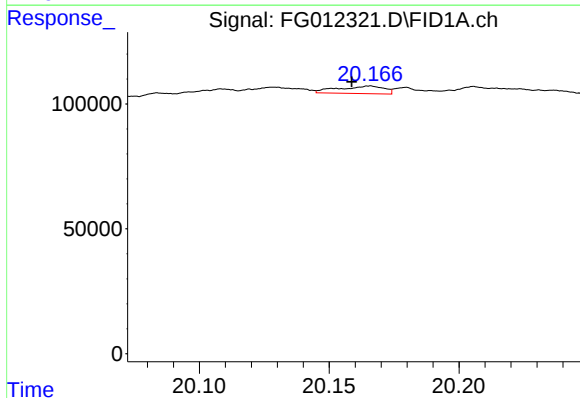

#21 n-Octatriacontane (C38)

R.T.: 20.166 min
Delta R.T.: 0.007 min
Response: 37170
Conc: 0.33 ug/ml

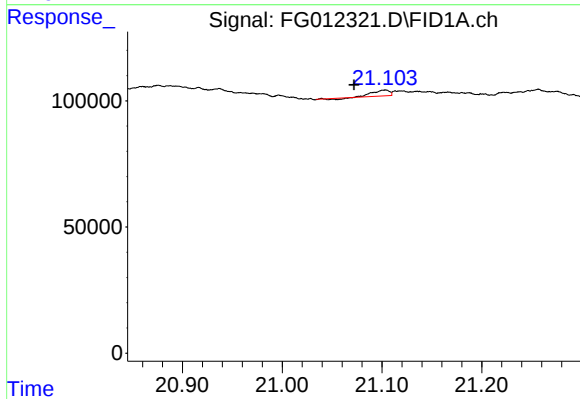

#22 n-Tetracontane (C40)

R.T.: 21.103 min
Delta R.T.: 0.031 min
Response: 23076
Conc: 0.20 ug/ml