

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG070522\  
Data File : FG010073.D  
Signal(s) : FID1A.ch  
Acq On : 05 Jul 2022 10:30  
Operator : AJ\MA  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 06 01:40:45 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG062922.M  
Quant Title :  
QLast Update : Thu Jun 30 04:15:08 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.512  | 2463309  | 19.058 ug/ml |
| 12)                         | N-OCTACOSANE | 16.988 | 2387445  | 18.589 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG070522\  
Data File : FG010073.D  
Signal(s) : FID1A.ch  
Acq On : 05 Jul 2022 10:30  
Operator : AJ\MA  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
RT MARKER

Integration File: autoint1.e  
Quant Time: Jul 06 01:40:45 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG062922.M  
Quant Title :  
QLast Update : Thu Jun 30 04:15:08 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

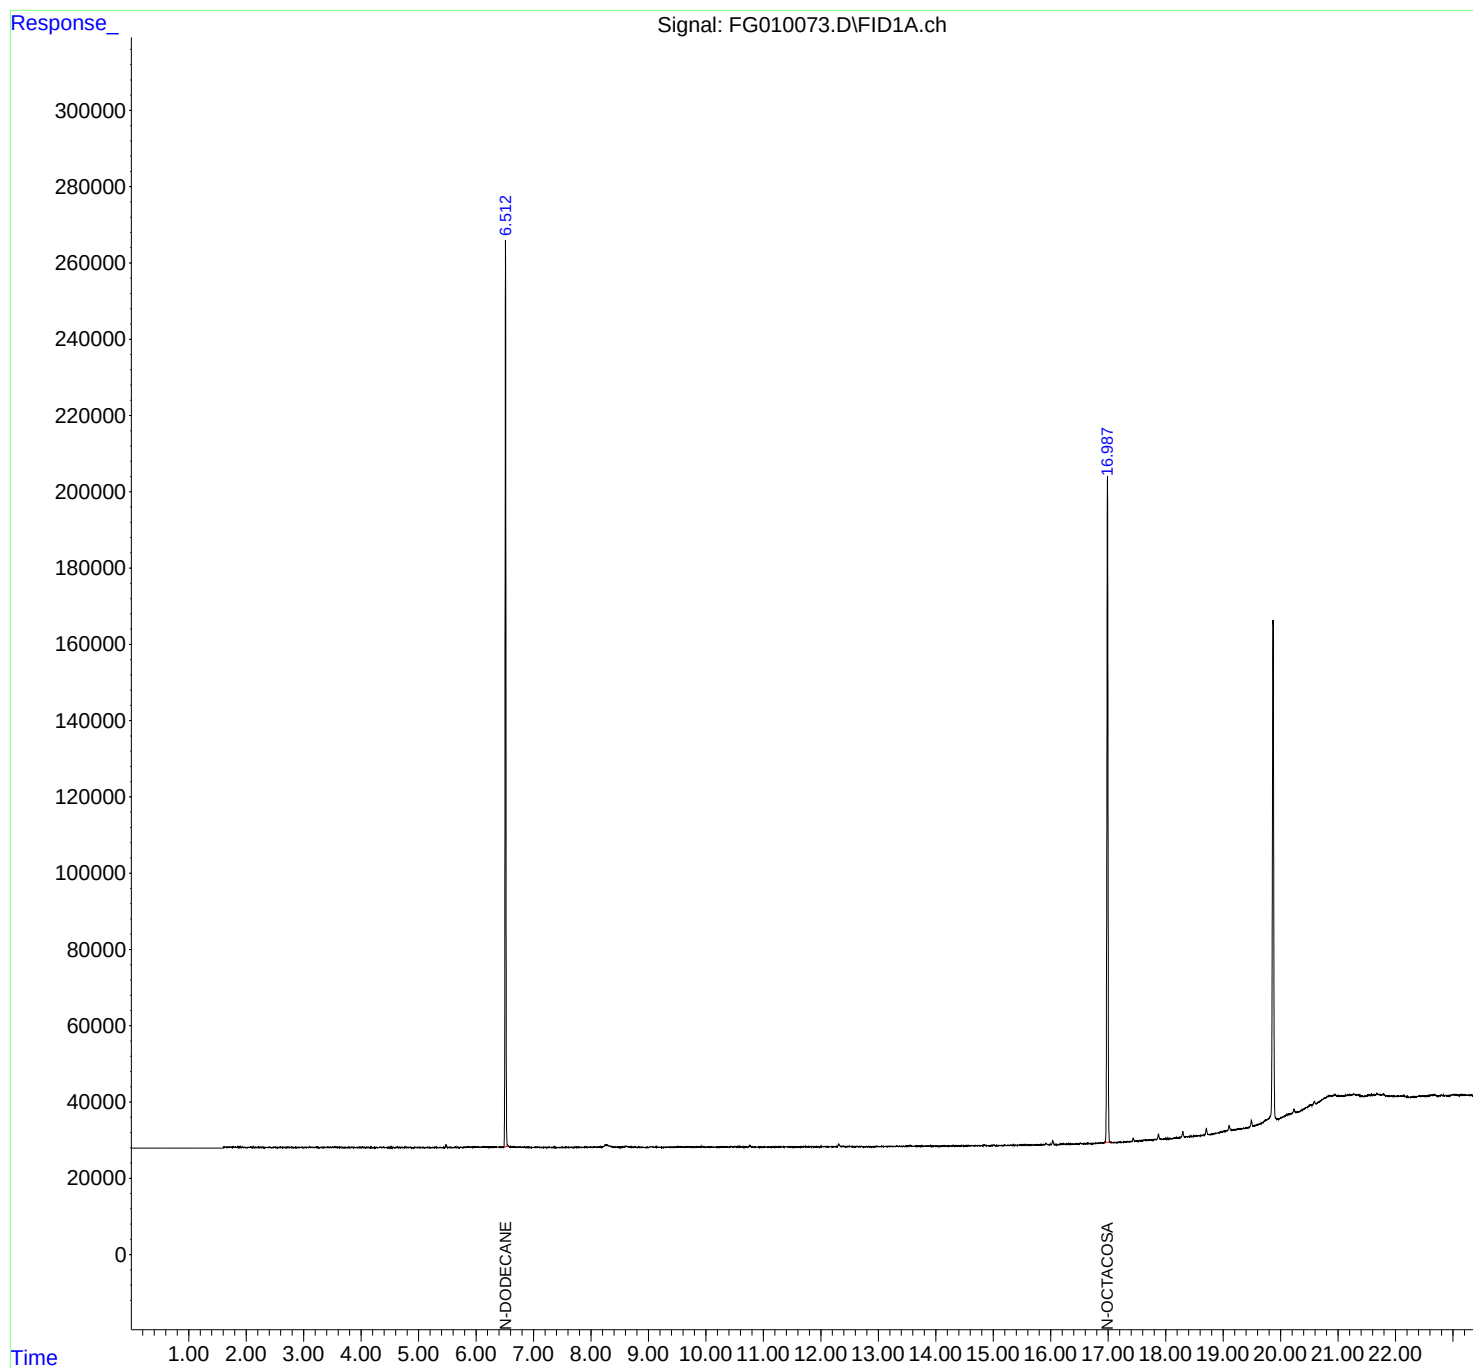


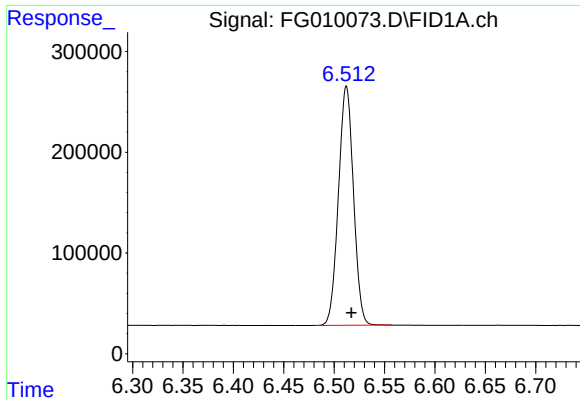

#3 N-DODECANE


R.T.: 6.512 min  
Delta R.T.: -0.005 min  
Response: 2463309  
Conc: 19.06 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
RT MARKER

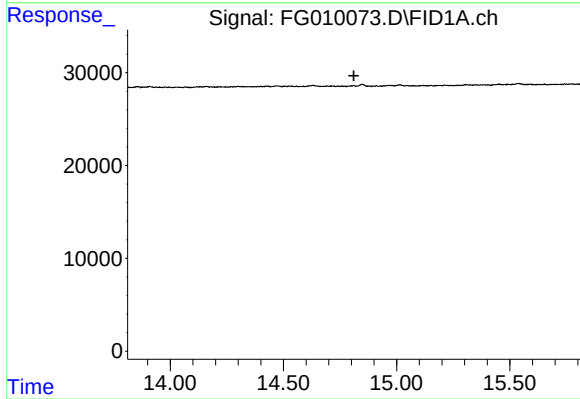

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.811 min  
Response: 0  
Conc: N.D.

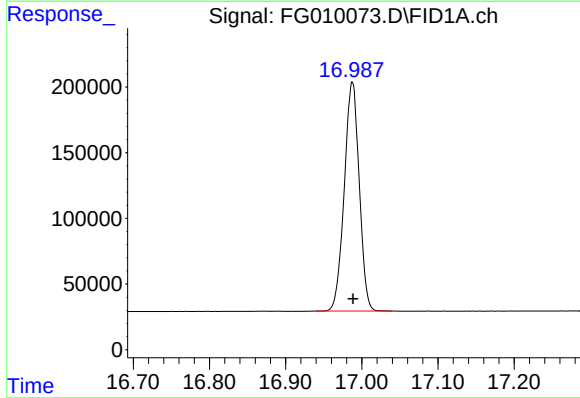

#12 N-OCTACOSANE

R.T.: 16.988 min  
Delta R.T.: -0.001 min  
Response: 2387445  
Conc: 18.59 ug/ml