

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG070722\  
 Data File : FG010104.D  
 Signal(s) : FID1A.ch  
 Acq On : 07 Jul 2022 12:30  
 Operator : AJ\MA  
 Sample : PB145927BL  
 Misc :  
 ALS Vial : 55 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 08 02:32:39 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG062922.M  
 Quant Title :  
 QLast Update : Thu Jun 30 04:15:08 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.805 | 2306846  | 19.401 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 17.869 | 24619    | 0.196 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.703 | 28045    | 0.237 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.487 | 23902    | 0.225 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG070722\  
Data File : FG010104.D  
Signal(s) : FID1A.ch  
Acq On : 07 Jul 2022 12:30  
Operator : AJ\MA  
Sample : PB145927BL  
Misc :  
ALS Vial : 55 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 08 02:32:39 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG062922.M  
Quant Title :  
QLast Update : Thu Jun 30 04:15:08 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

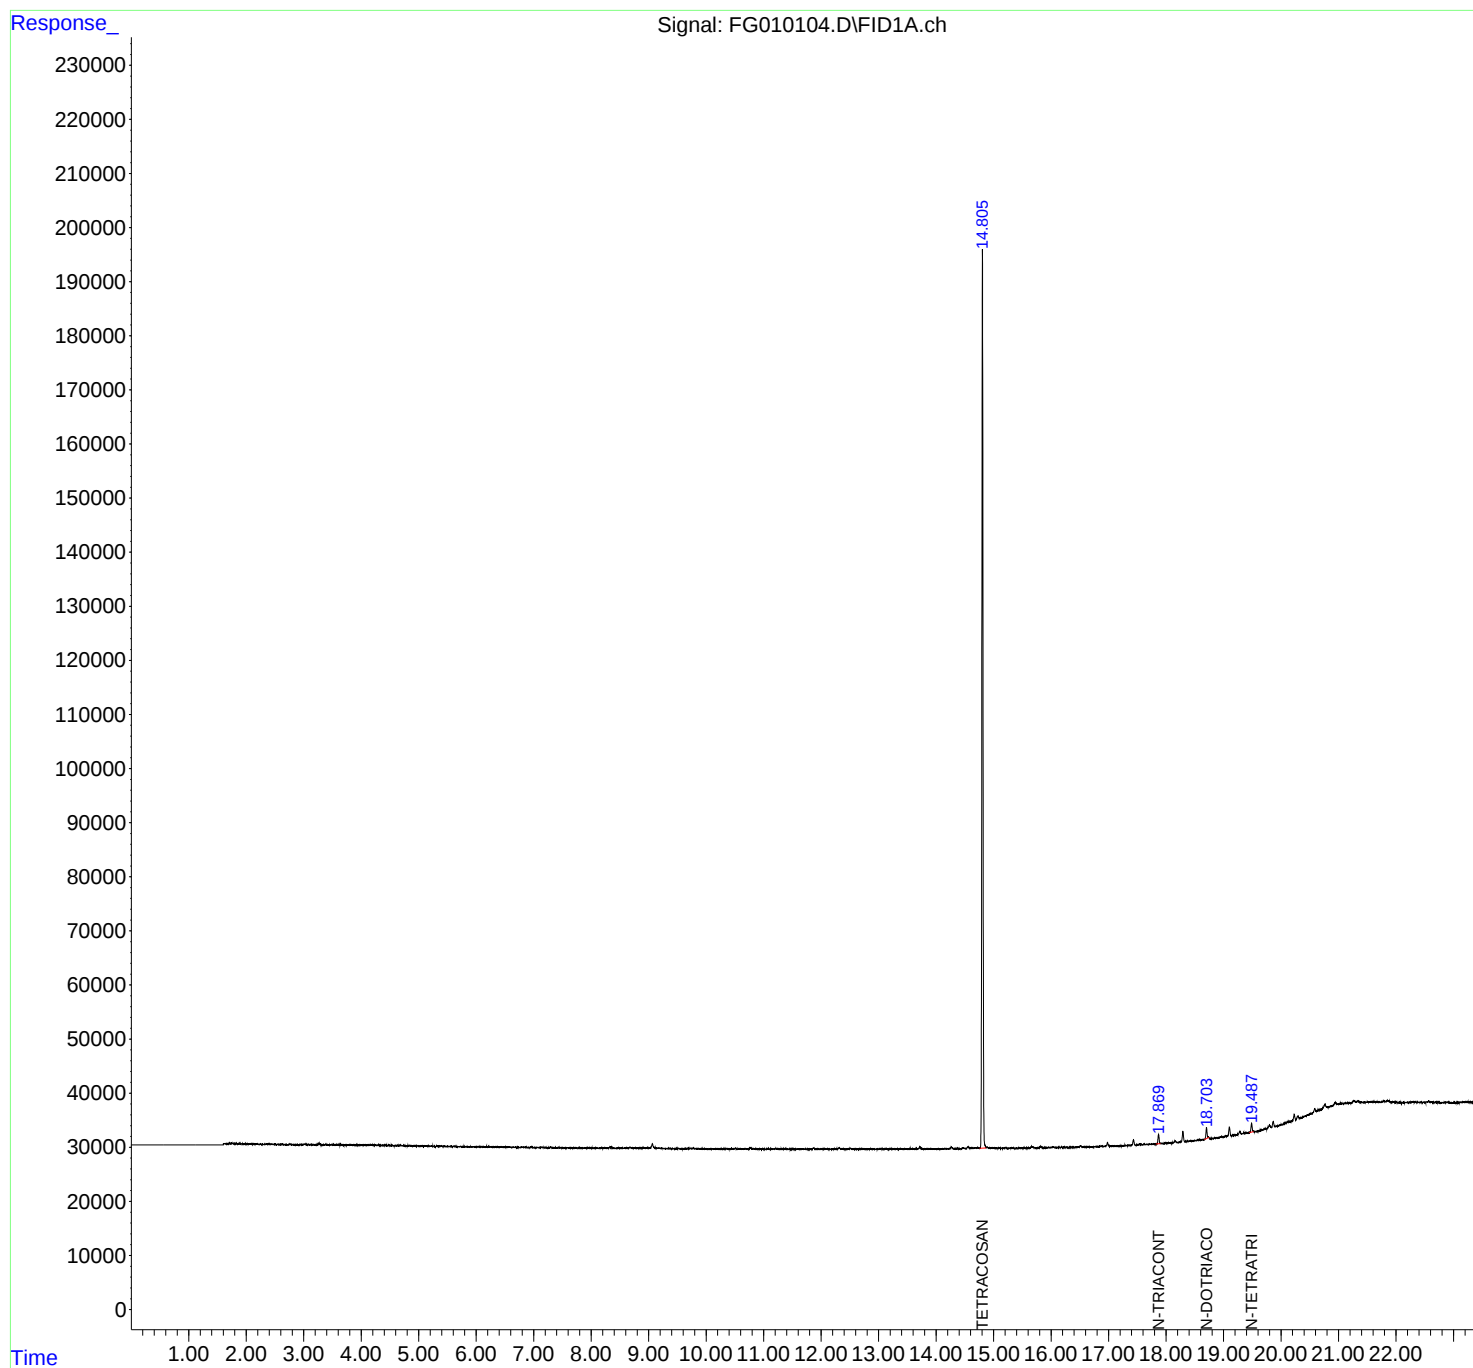


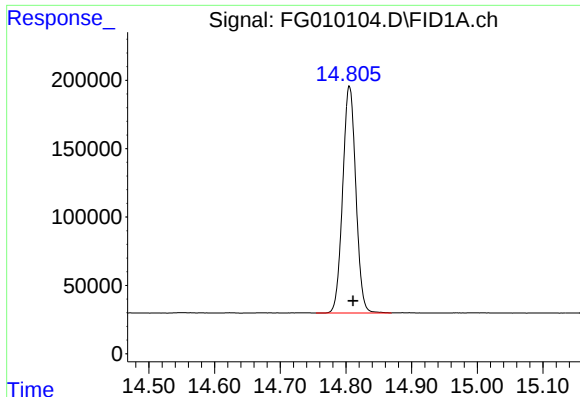

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.805 min  
Delta R.T.: -0.006 min  
Response: 2306846  
Conc: 19.40 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

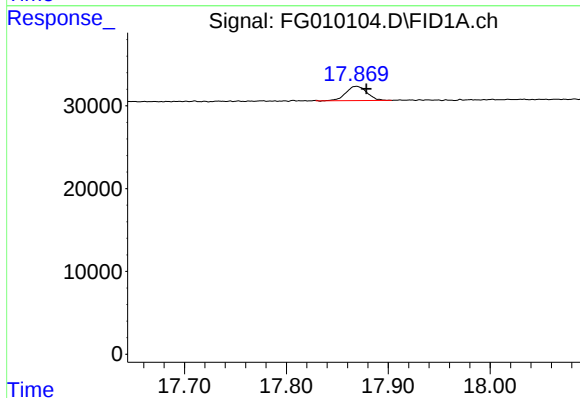


#13 N-TRIACONTANE

R.T.: 17.869 min  
Delta R.T.: -0.010 min  
Response: 24619  
Conc: 0.20 ug/ml

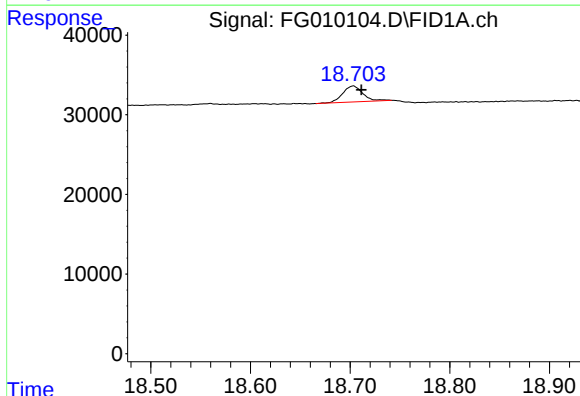

#14 N-DOTRIACONTANE

R.T.: 18.703 min  
Delta R.T.: -0.008 min  
Response: 28045  
Conc: 0.24 ug/ml

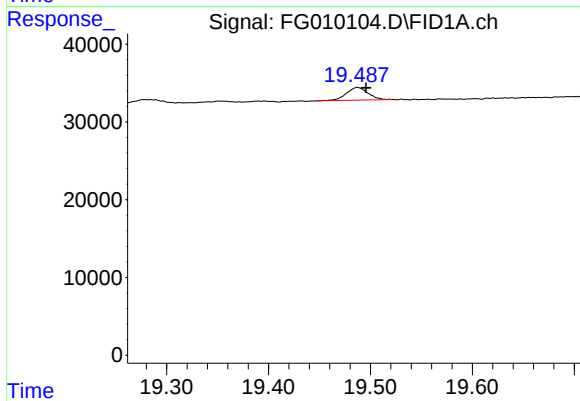

#15 N-TETRATRIACONTANE

R.T.: 19.487 min  
Delta R.T.: -0.008 min  
Response: 23902  
Conc: 0.22 ug/ml