

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070722\
 Data File : FG010107.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jul 2022 14:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 08 02:33:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
 Quant Title :
 QLast Update : Thu Jun 30 04:15:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.807	2283019	19.200 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.870	43034	0.342 ug/ml
14) N-DOTRIACONTANE	18.701	55795	0.472 ug/ml
15) N-TETRATRIACONTANE	19.488	43898	0.413 ug/ml
16) N-HEXATRIACONTANE	20.227	29371	0.330 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070722\
Data File : FG010107.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2022 14:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 02:33:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

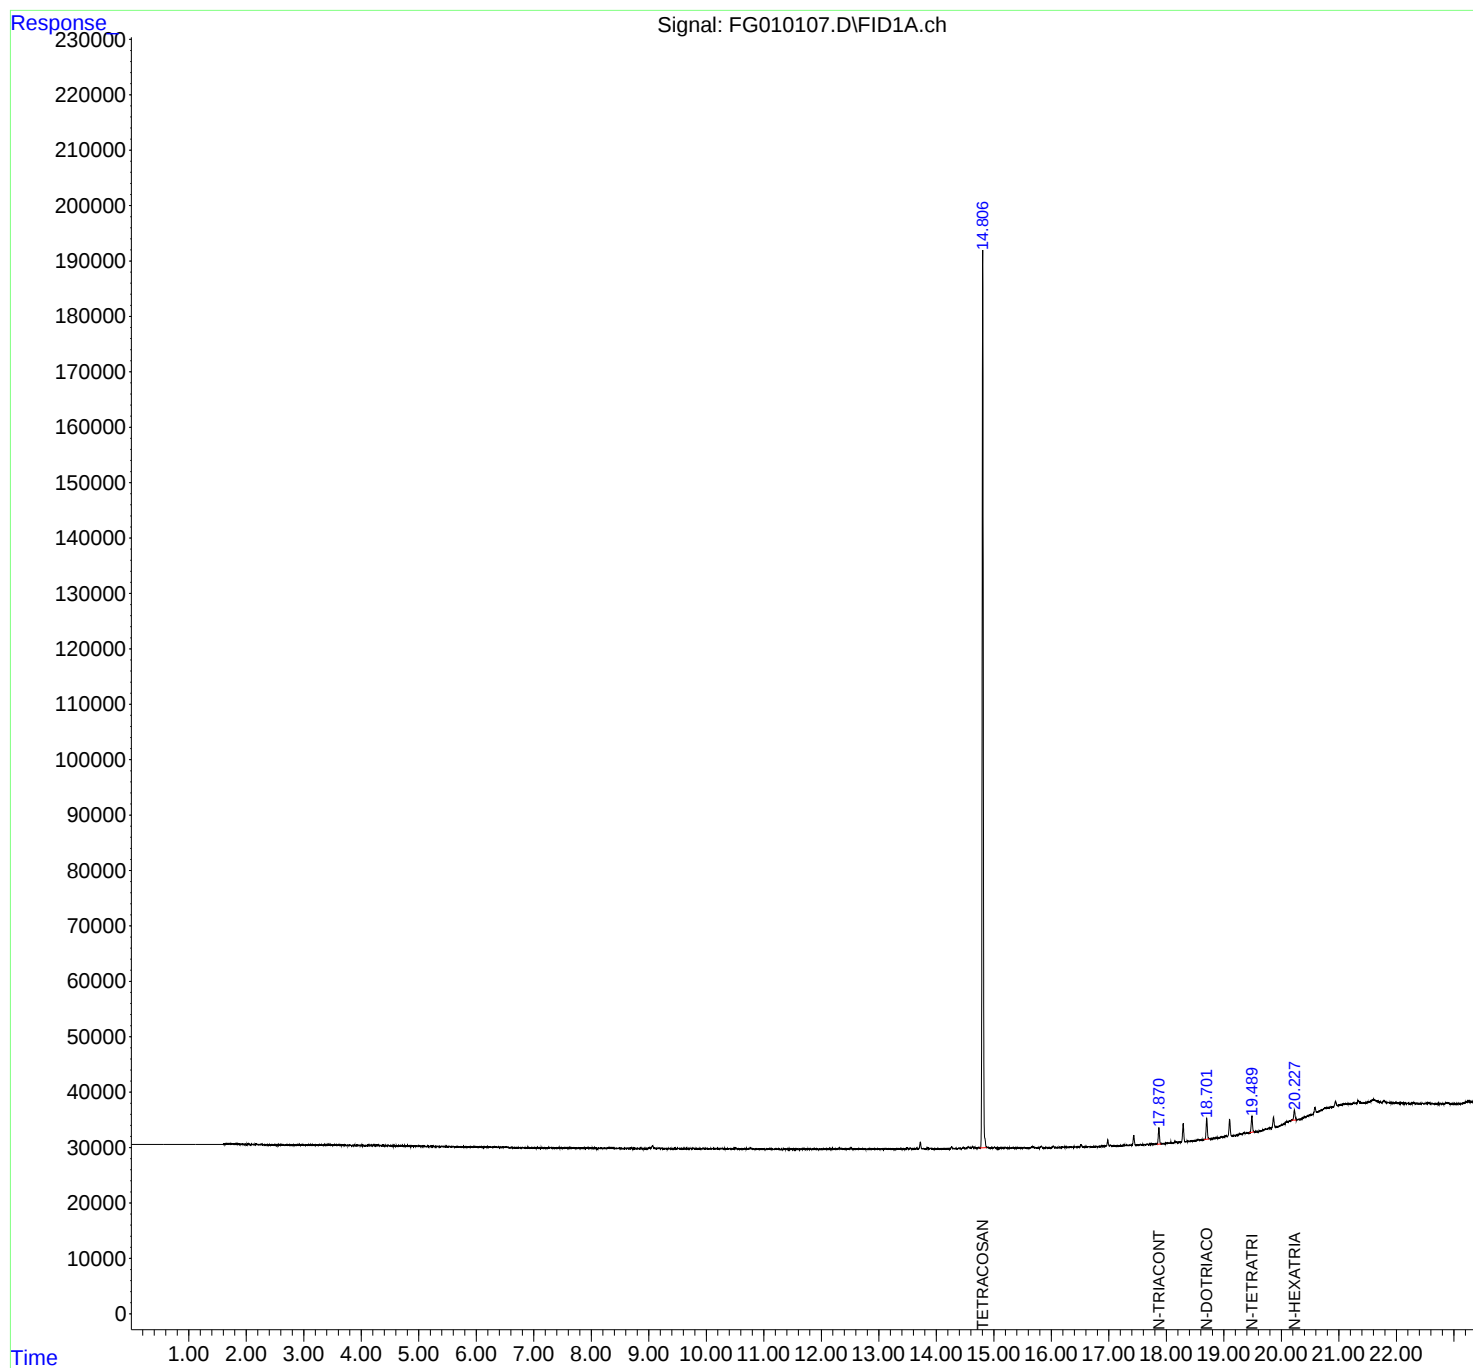


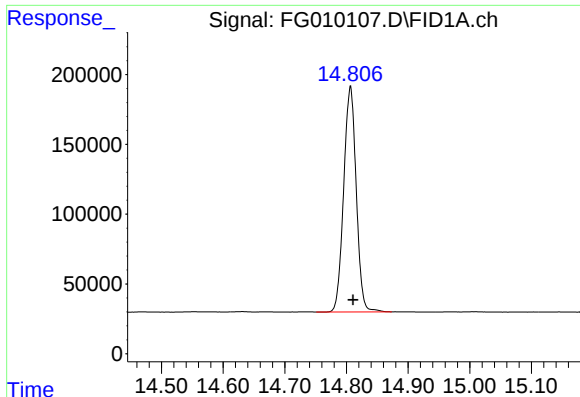

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.807 min
Delta R.T.: -0.004 min
Response: 2283019
Conc: 19.20 ug/ml

Instrument :
FID_G
ClientSampleId :

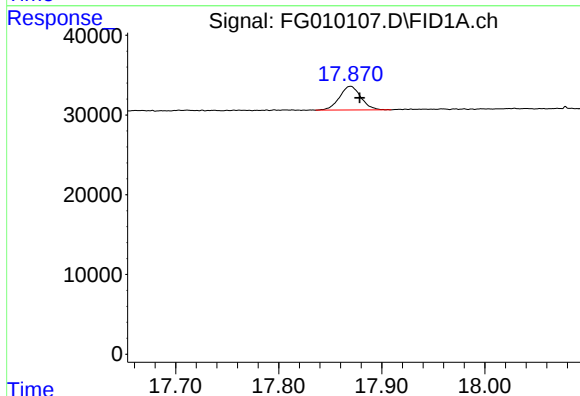


#13 N-TRIACONTANE

R.T.: 17.870 min
Delta R.T.: -0.009 min
Response: 43034
Conc: 0.34 ug/ml

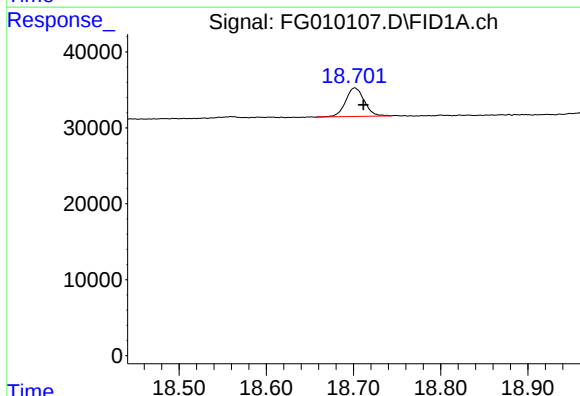


#14 N-DOTRIACONTANE

R.T.: 18.701 min
Delta R.T.: -0.010 min
Response: 55795
Conc: 0.47 ug/ml

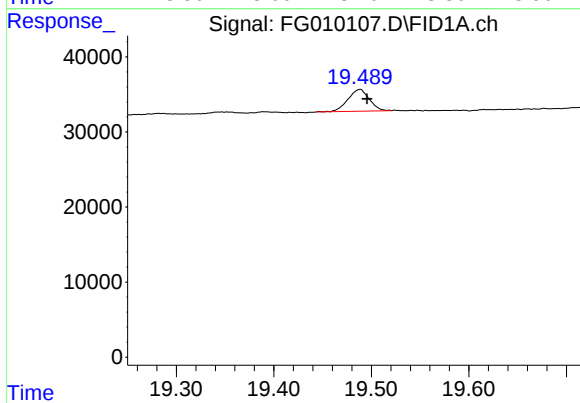

#15 N-TETRATRIACONTANE

R.T.: 19.488 min
Delta R.T.: -0.007 min
Response: 43898
Conc: 0.41 ug/ml

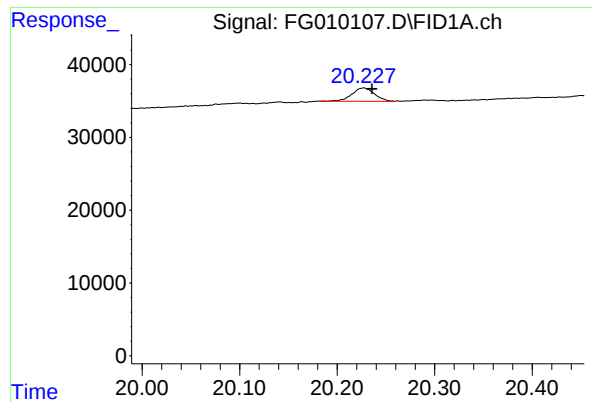

#16 N-HEXATRIACONTANE

R.T.: 20.227 min
Delta R.T.: -0.008 min
Response: 29371
Conc: 0.33 ug/ml

Instrument :

FID_G

ClientSampleId :