

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070722\
Data File : FG010118.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2022 20:18
Operator : AJ\MA
Sample : N3581-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-6-070522

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2022
Supervised By :Ankita Jodhani 07/08/2022

Integration File: autoint1.e
Quant Time: Jul 08 02:35:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.808	135736	1.142 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070722\
Data File : FG010118.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2022 20:18
Operator : AJ\MA
Sample : N3581-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
AU-6-070522


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2022
Supervised By :Ankita Jodhani 07/08/2022

Integration File: autoint1.e
Quant Time: Jul 08 02:35:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

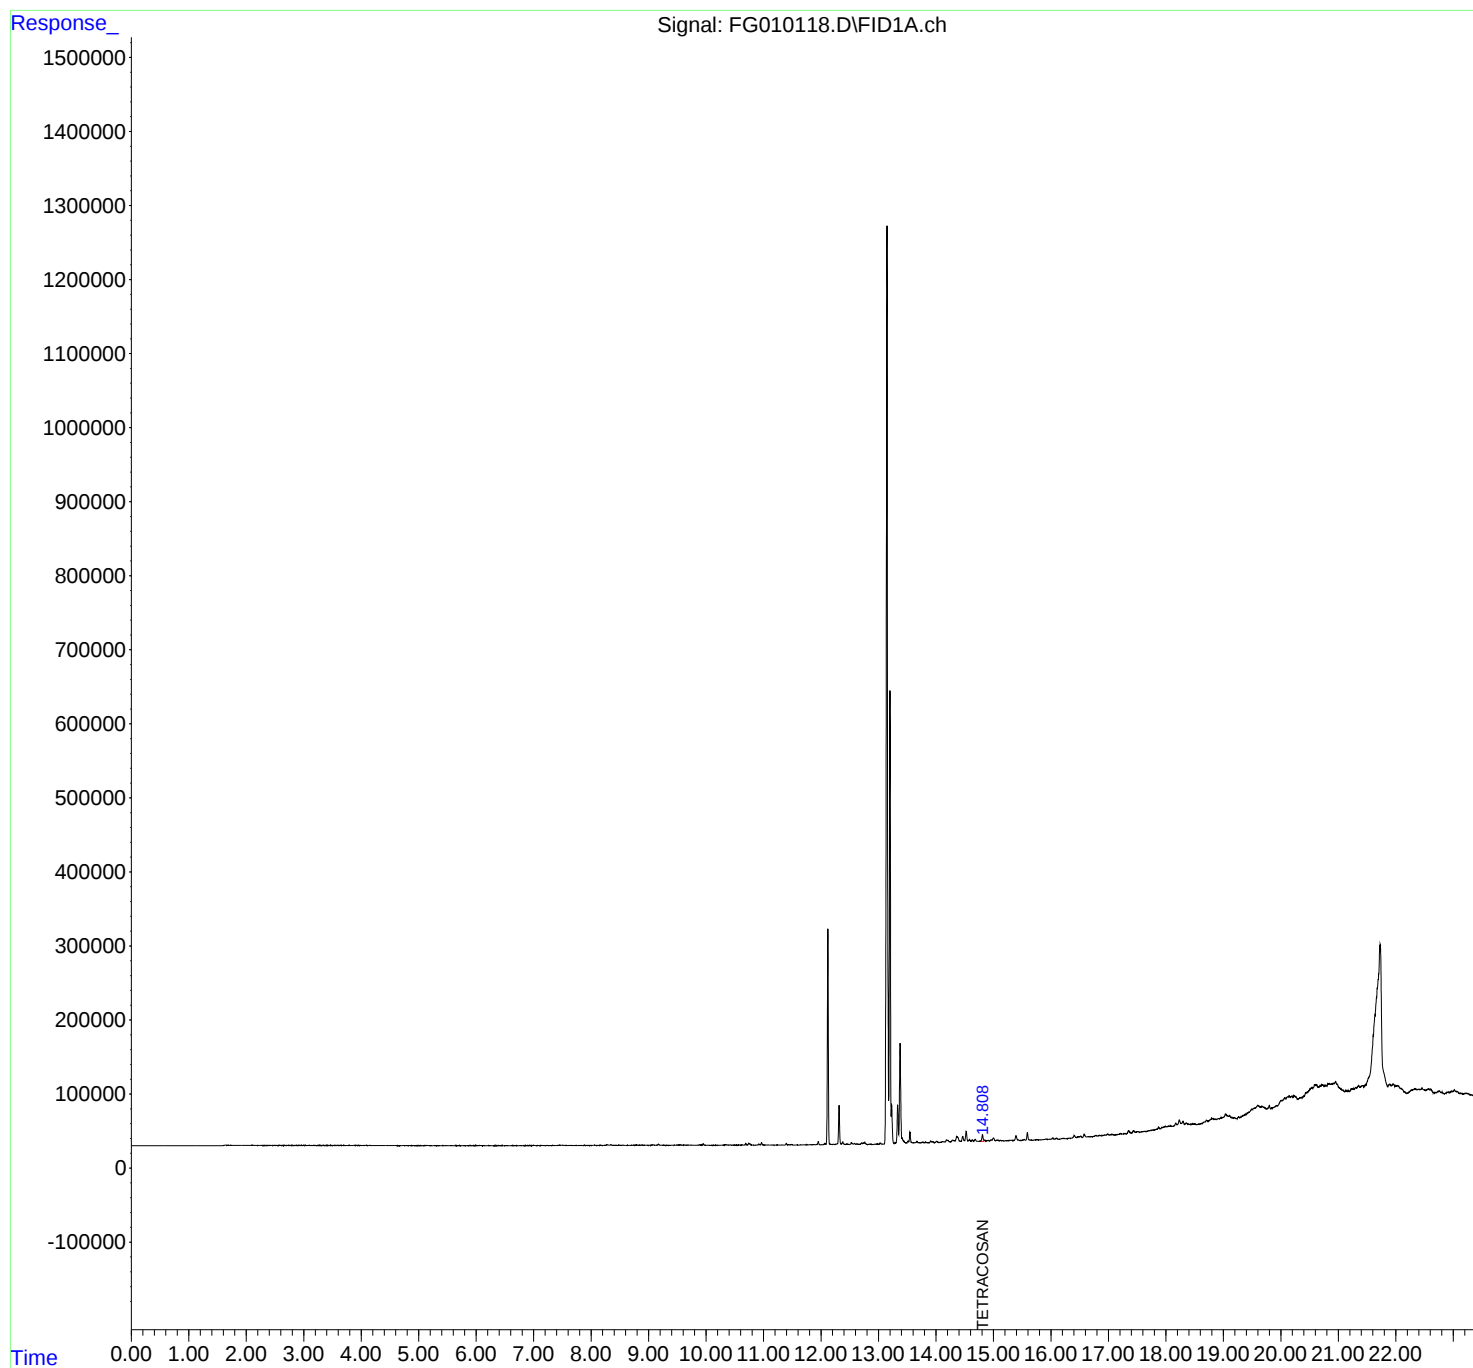

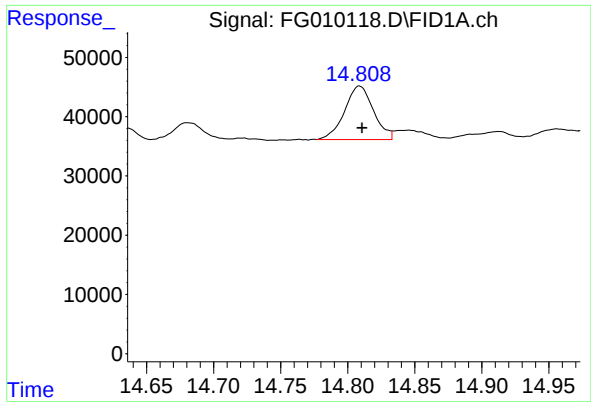

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.808 min
Delta R.T.: -0.003 min
Response: 135736
Conc: 1.14 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-6-070522

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2022
Supervised By :Ankita Jodhani 07/08/2022