

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
 Data File : FG012341.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jul 2023 11:07
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 08 00:34:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
 Quant Title :
 QLast Update : Thu Jul 06 13:57:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.984	2236493	20.928 ug/ml
Target Compounds				
10)	N-TETRACOSANE	15.166	160217	1.211 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
Data File : FG012341.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2023 11:07
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 00:34:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

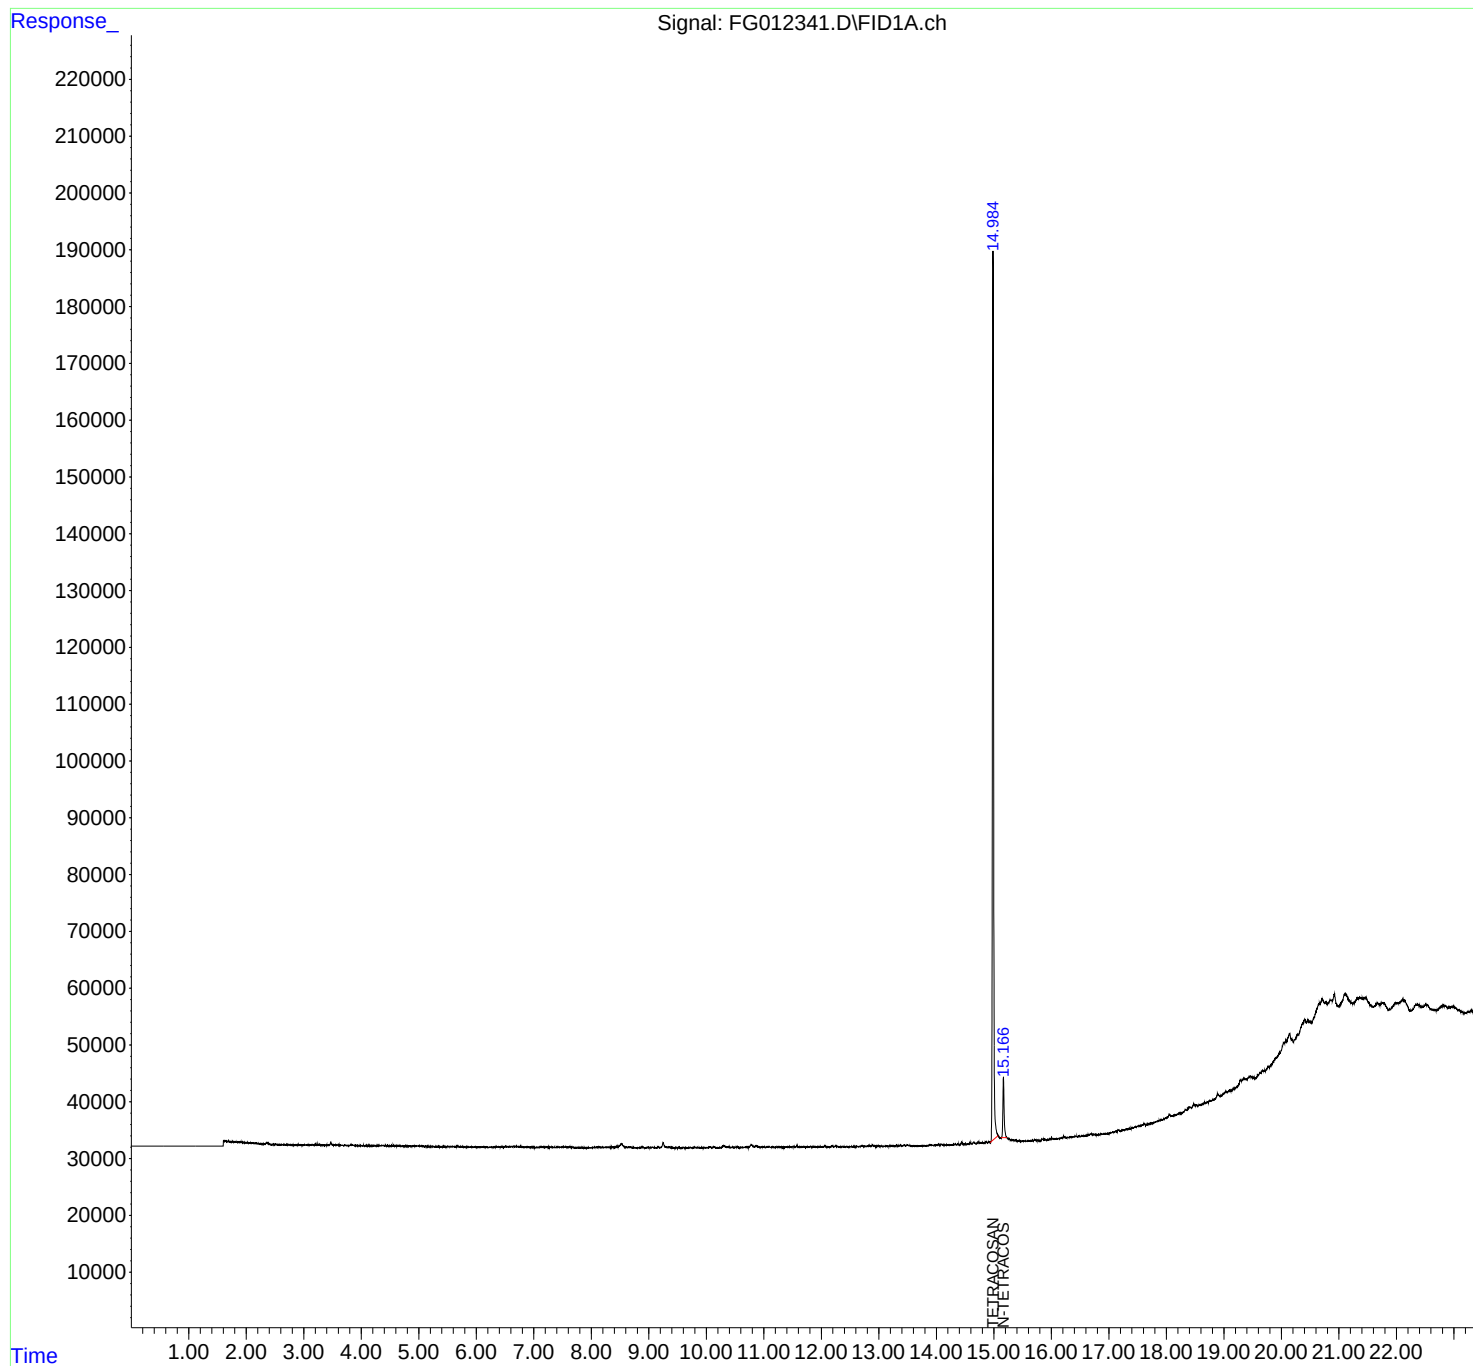


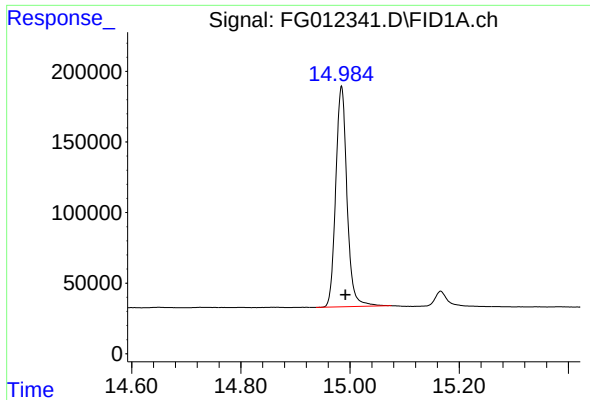

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.984 min
Delta R.T.: -0.007 min
Response: 2236493
Conc: 20.93 ug/ml

Instrument :
FID_G
ClientSampleId :

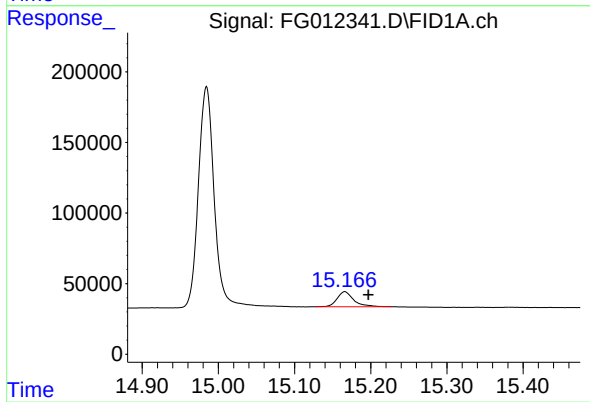

#10 N-TETRACOSANE

R.T.: 15.166 min
Delta R.T.: -0.031 min
Response: 160217
Conc: 1.21 ug/ml