

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
 Data File : FG012357.D
 Signal(s) : FID1A.ch
 Acq On : 07 Jul 2023 19:47
 Operator : YP\AJ
 Sample : 03510-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 08 00:40:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
 Quant Title :
 QLast Update : Thu Jul 06 13:57:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.982	1526871	14.288 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.165	250018	1.890 ug/ml
11) N-HEXACOSANE	16.208	51970	0.444 ug/ml
12) N-OCTACOSANE	17.159	76999	0.674 ug/ml
13) N-TRIACONTANE	18.047	110425	0.996 ug/ml
14) N-DOTRIACONTANE	18.880	53575	0.513 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
Data File : FG012357.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2023 19:47
Operator : YP\AJ
Sample : 03510-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 00:40:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

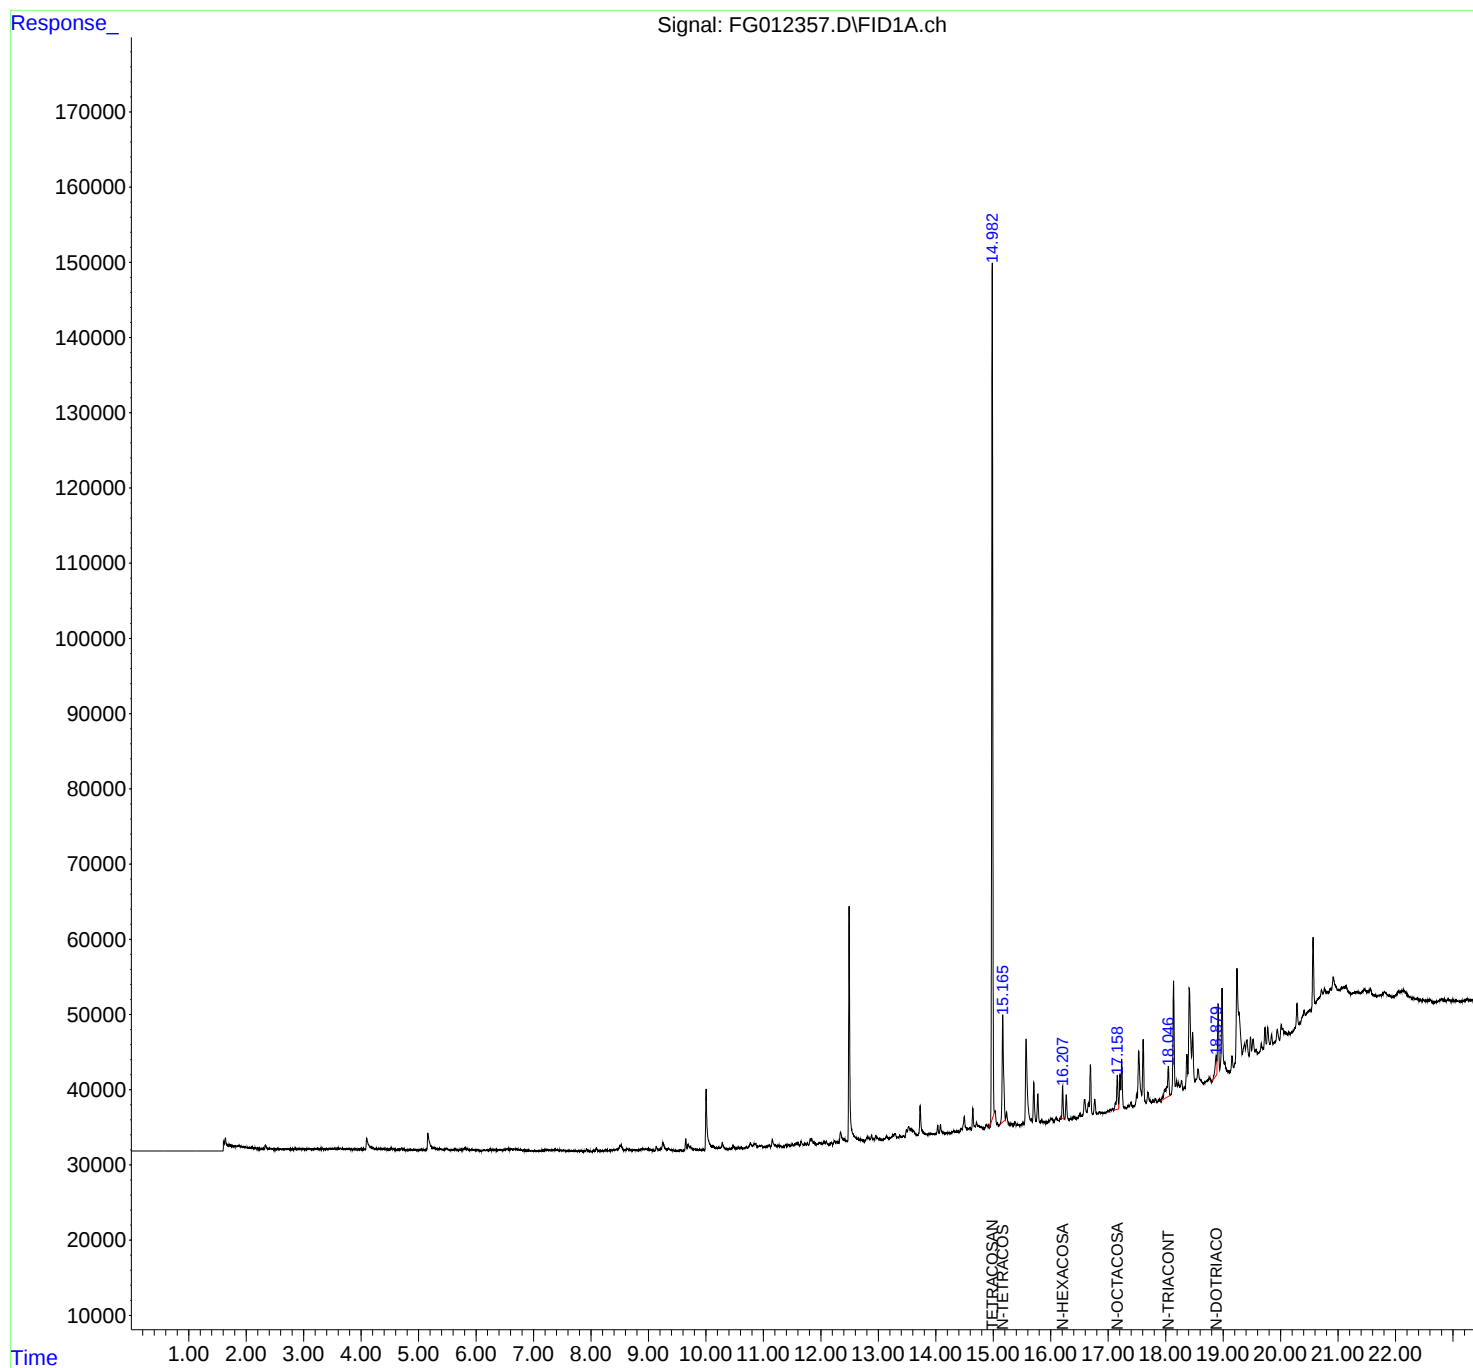


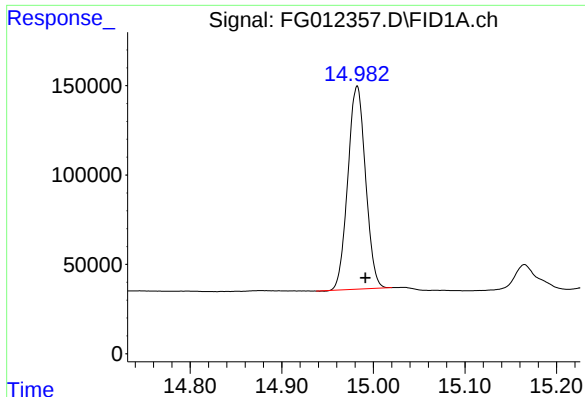

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.982 min
Delta R.T.: -0.009 min
Response: 1526871
Conc: 14.29 ug/ml

Instrument :
FID_G
ClientSampleId :

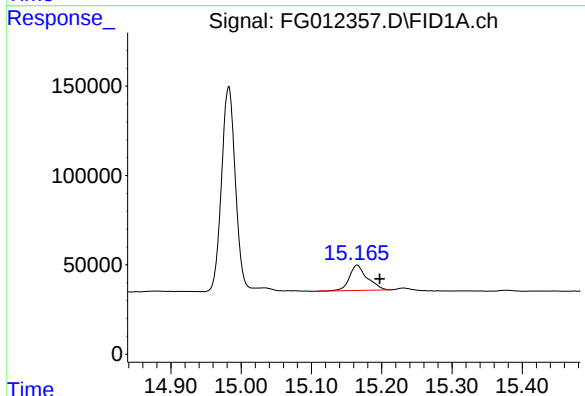


#10 N-TETRACOSANE

R.T.: 15.165 min
Delta R.T.: -0.032 min
Response: 250018
Conc: 1.89 ug/ml

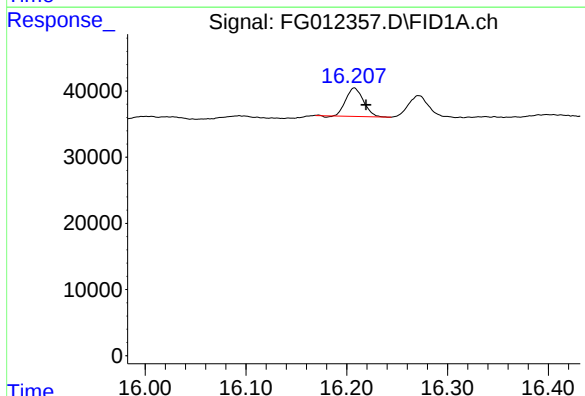


#11 N-HEXACOSANE

R.T.: 16.208 min
Delta R.T.: -0.012 min
Response: 51970
Conc: 0.44 ug/ml

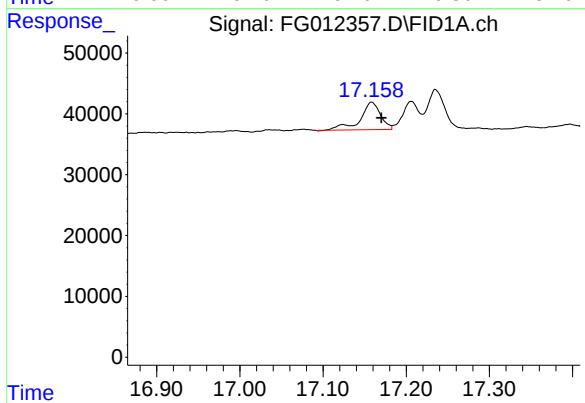

#12 N-OCTACOSANE


R.T.: 17.159 min
Delta R.T.: -0.011 min
Response: 76999
Conc: 0.67 ug/ml

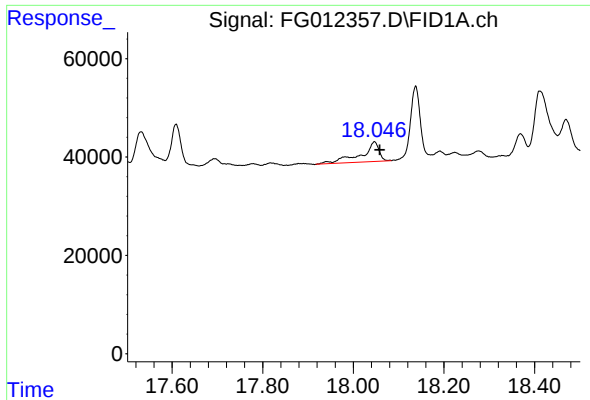

#13 N-TRIACONTANE

R.T.: 18.047 min
Delta R.T.: -0.012 min
Response: 110425
Conc: 1.00 ug/ml

Instrument :
FID_G
ClientSampleId :

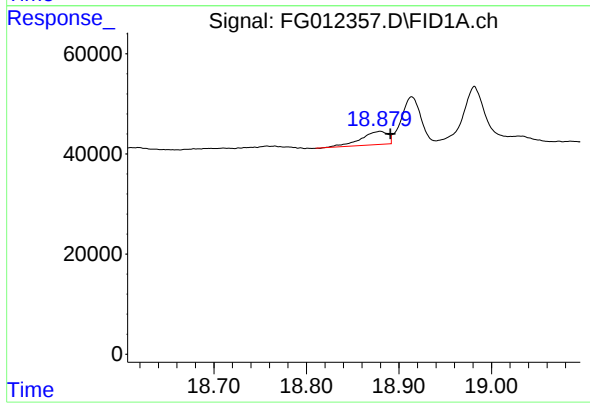

#14 N-DOTRIACONTANE

R.T.: 18.880 min
Delta R.T.: -0.011 min
Response: 53575
Conc: 0.51 ug/ml