

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
Data File : FG012361.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2023 21:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 00:41:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.982	1892856	17.713 ug/ml
Target Compounds				
10)	N-TETRACOSANE	15.165	176477	1.334 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
Data File : FG012361.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2023 21:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 08 00:41:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

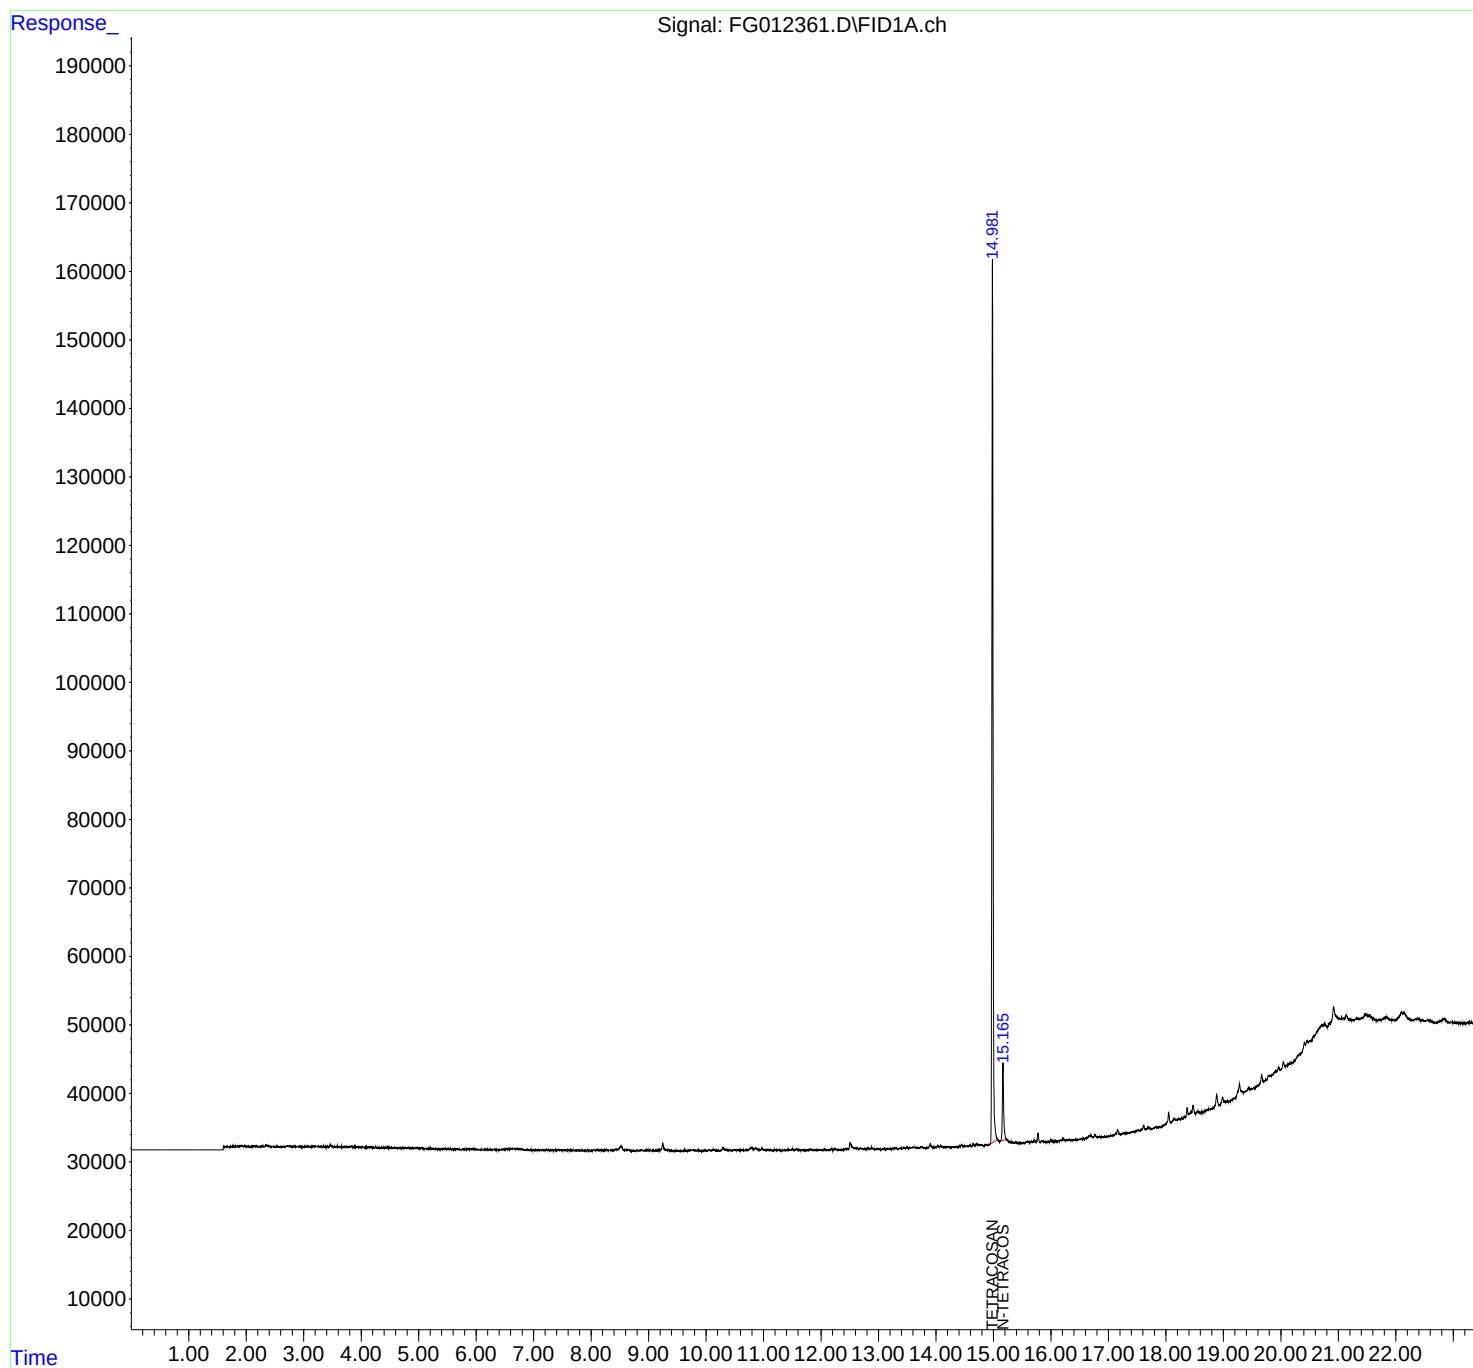


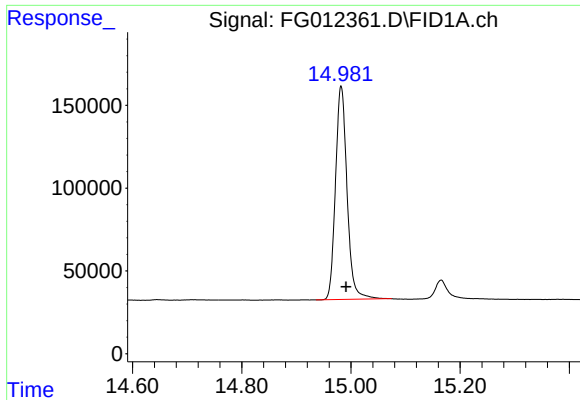

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.982 min
Delta R.T.: -0.009 min
Response: 1892856
Conc: 17.71 ug/ml

Instrument :
FID_G
ClientSampleId :

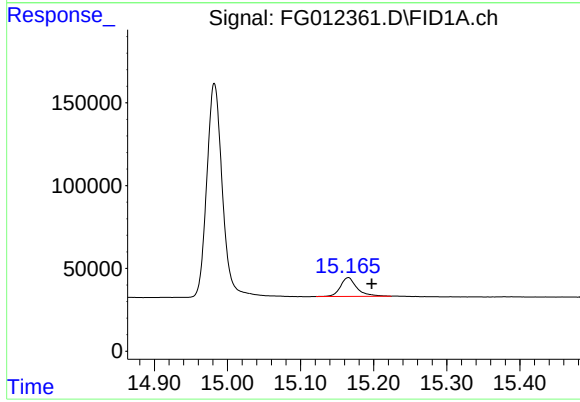

#10 N-TETRACOSANE

R.T.: 15.165 min
Delta R.T.: -0.032 min
Response: 176477
Conc: 1.33 ug/ml