

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
Data File : FG012356.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2023 19:17
Operator : YP\AJ
Sample : 03510-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC-WWS-07-G

Integration File: autoint1.e
Quant Time: Jul 08 00:39:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.983	2388962	22.355 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070723\
Data File : FG012356.D
Signal(s) : FID1A.ch
Acq On : 07 Jul 2023 19:17
Operator : YP\AJ
Sample : 03510-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC-WWS-07-G

Integration File: autoint1.e
Quant Time: Jul 08 00:39:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

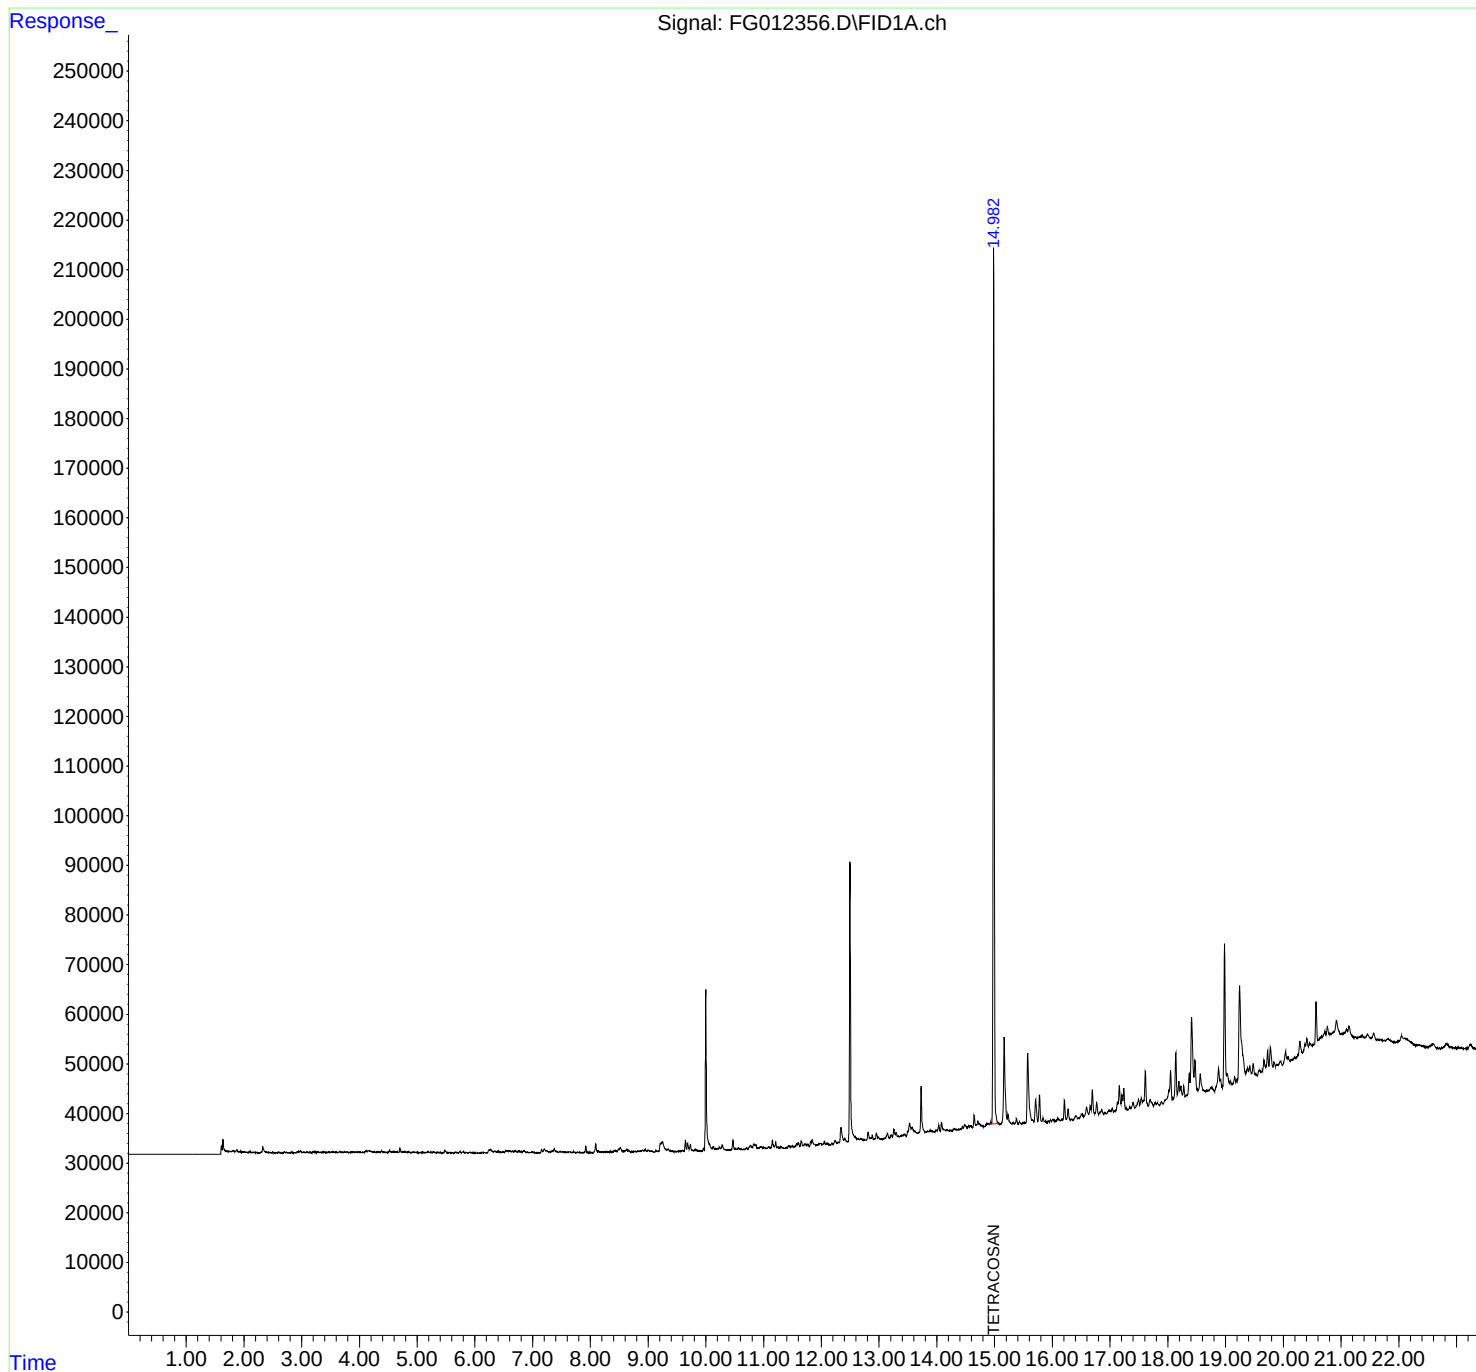

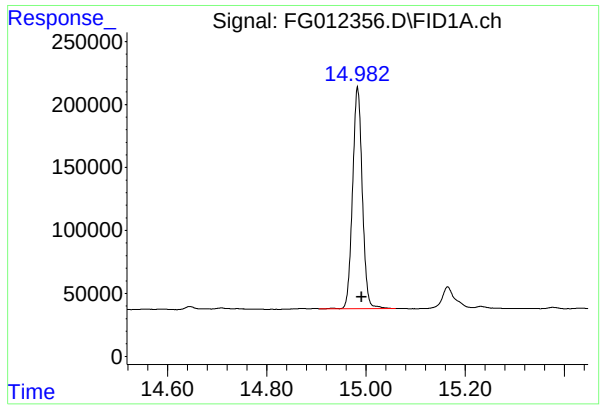

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.983 min
Delta R.T.: -0.008 min
Response: 2388962
Conc: 22.35 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-WWS-07-G