

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071025\
Data File : FG016277.D
Signal(s) : FID1A.ch
Acq On : 10 Jul 2025 15:42
Operator : YP\AJ
Sample : Q2473-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PIT#1

Integration File: autoint1.e
Quant Time: Jul 11 04:14:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070925.M
Quant Title :
QLast Update : Wed Jul 09 12:46:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.201	149654	1.497 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071025\
Data File : FG016277.D
Signal(s) : FID1A.ch
Acq On : 10 Jul 2025 15:42
Operator : YP\AJ
Sample : Q2473-01 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PIT#1

Integration File: autoint1.e
Quant Time: Jul 11 04:14:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070925.M
Quant Title :
QLast Update : Wed Jul 09 12:46:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

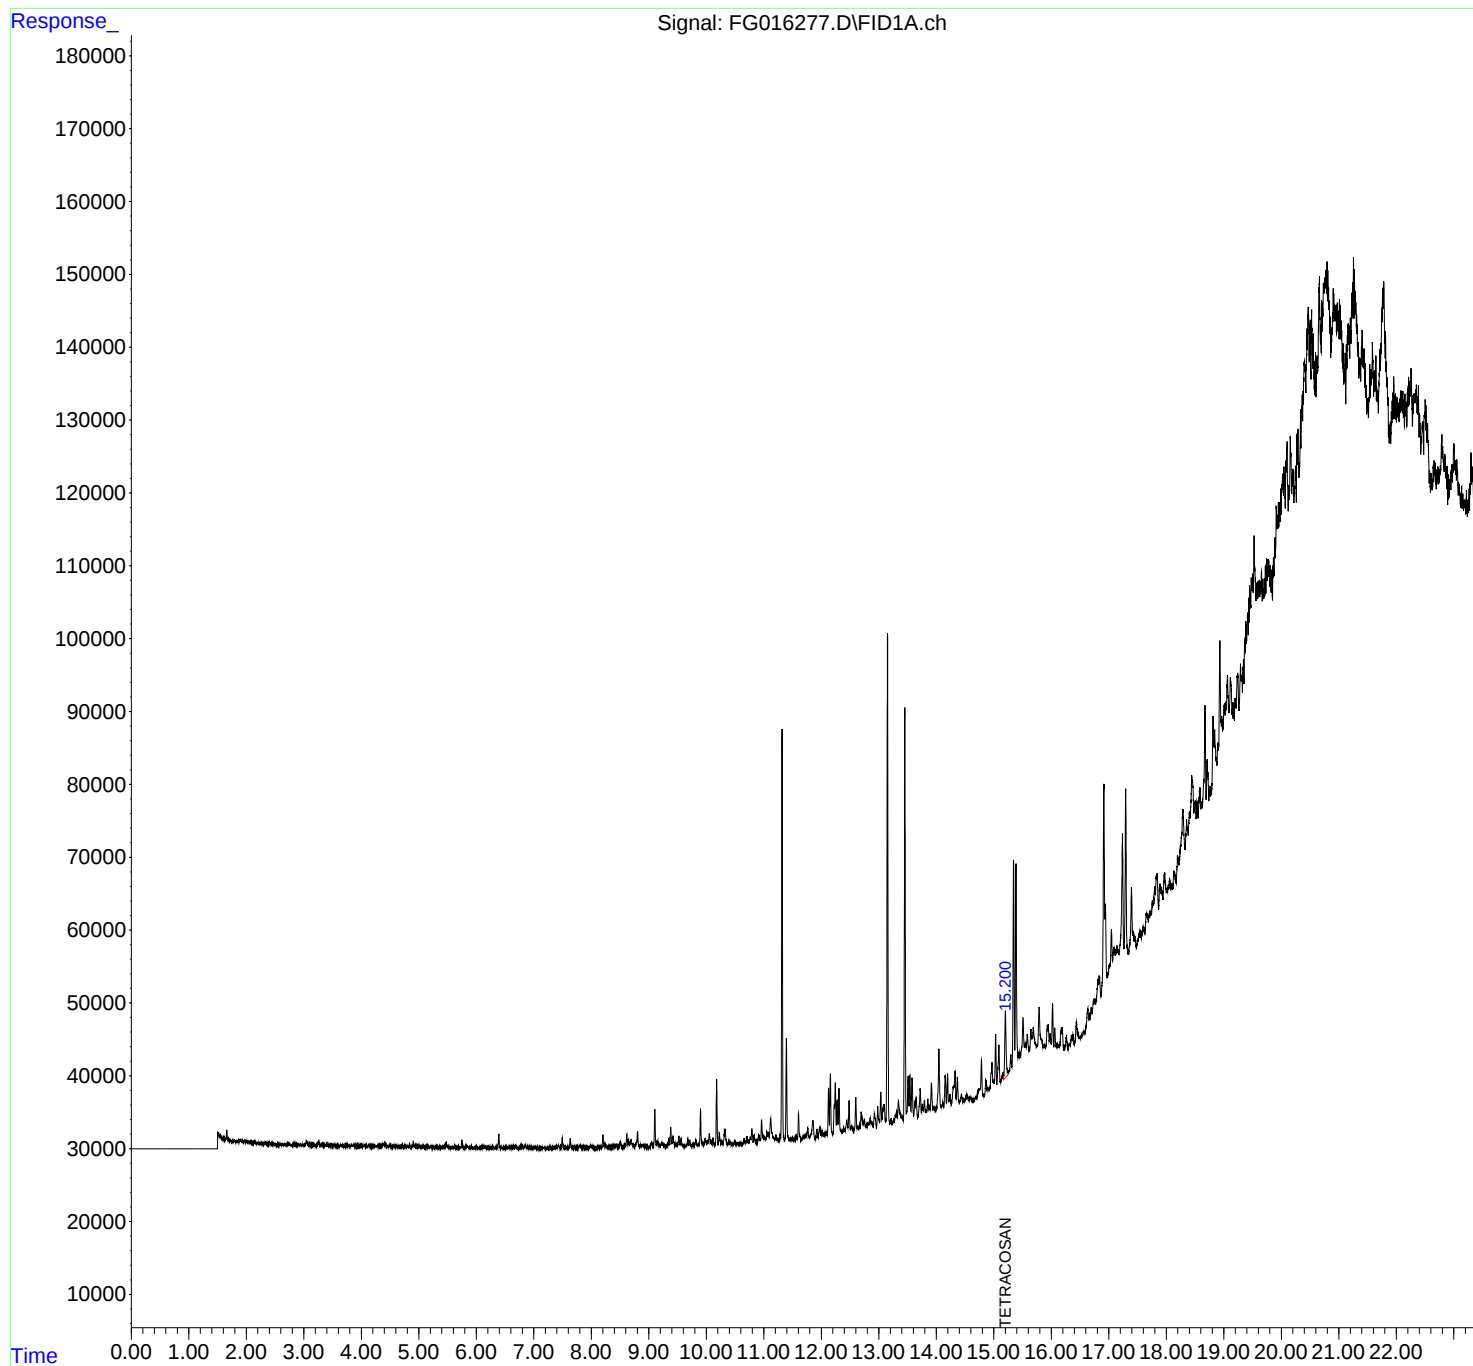

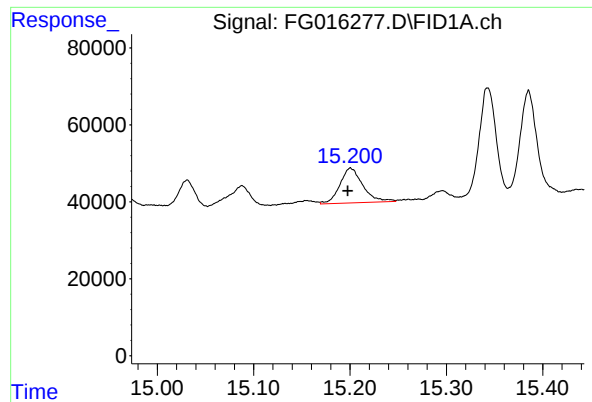

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.201 min
Delta R.T.: 0.003 min
Response: 149654
Conc: 1.50 ug/ml

Instrument :
FID_G
ClientSampleId :
PIT#1