

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071223\
Data File : FG012367.D
Signal(s) : FID1A.ch
Acq On : 12 Jul 2023 12:58
Operator : YP\AJ
Sample : PB154130BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 01:17:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.982	1884485	17.634 ug/ml
Target Compounds				
10)	N-TETRACOSANE	15.164	113135	0.855 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071223\
Data File : FG012367.D
Signal(s) : FID1A.ch
Acq On : 12 Jul 2023 12:58
Operator : YP\AJ
Sample : PB154130BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 13 01:17:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

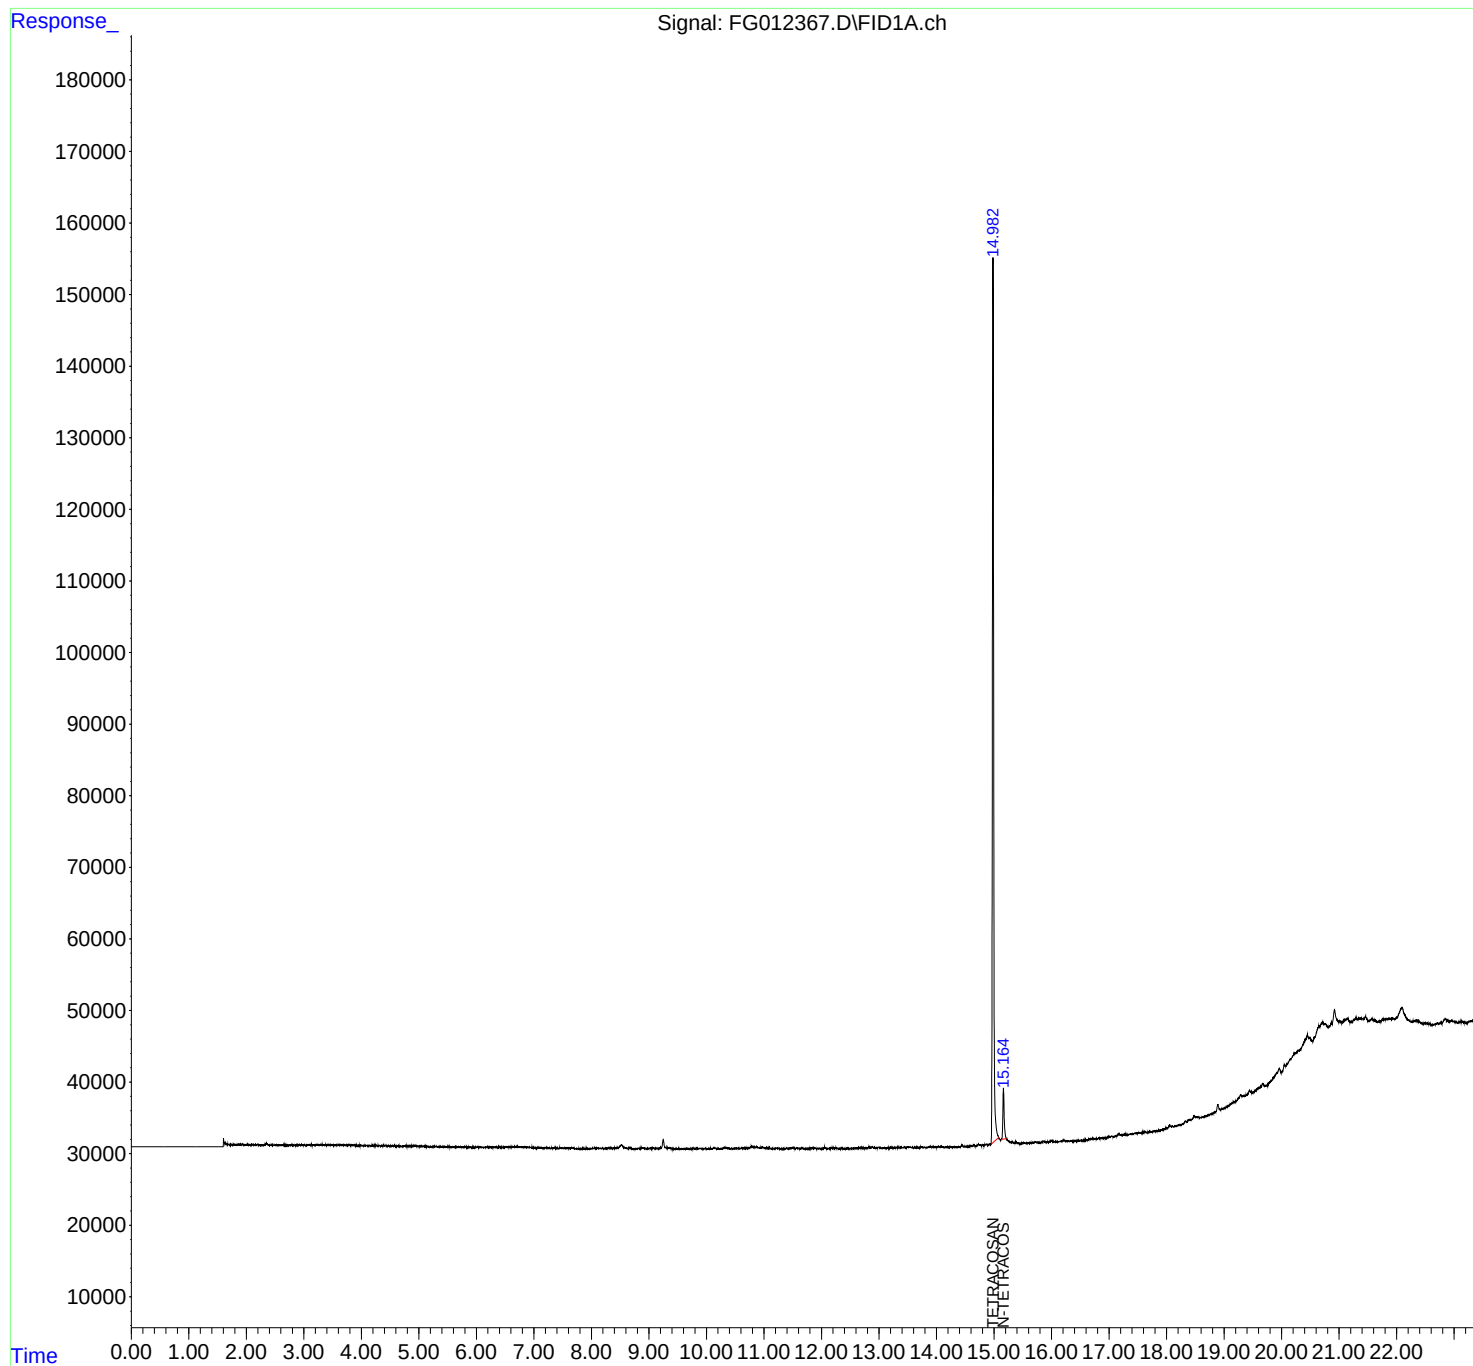


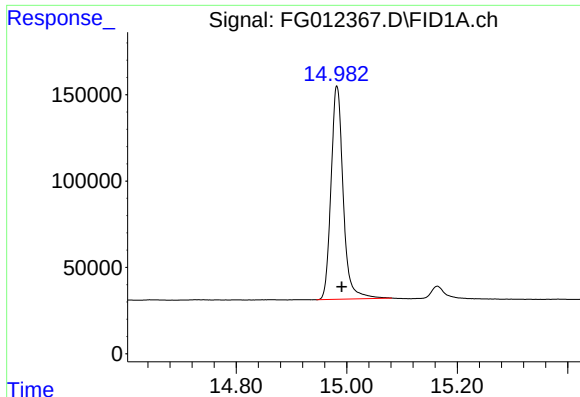

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.982 min
Delta R.T.: -0.009 min
Response: 1884485
Conc: 17.63 ug/ml

Instrument :
FID_G
ClientSampleId :

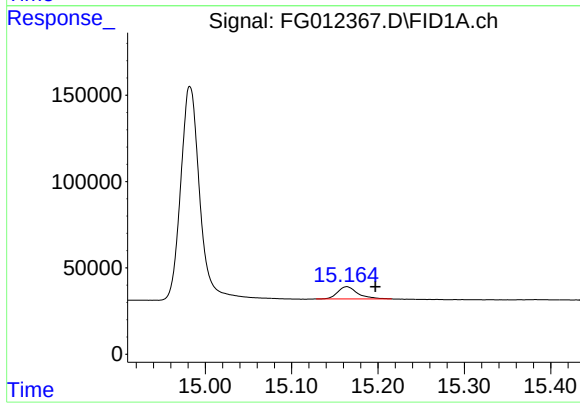

#10 N-TETRACOSANE

R.T.: 15.164 min
Delta R.T.: -0.033 min
Response: 113135
Conc: 0.86 ug/ml