

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071720\
 Data File : FG007081.D
 Signal(s) : FID1A.ch
 Acq On : 17 Jul 2020 15:30
 Operator : DD\AJ
 Sample : L3183-11 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 OK-03-071520

Integration File: autoint1.e
 Quant Time: Jul 18 02:07:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071520.M
 Quant Title :
 QLast Update : Thu Jul 16 02:29:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.637f	187764	1.007 ug/ml
8) N-DOCOSANE	13.921	351270	1.887 ug/ml
10) N-TETRACOSANE	14.977	1074139	5.747 ug/ml
12) N-OCTACOSANE	16.978	339512	1.843 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071720\
Data File : FG007081.D
Signal(s) : FID1A.ch
Acq On : 17 Jul 2020 15:30
Operator : DD\AJ
Sample : L3183-11 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-03-071520

Integration File: autoint1.e
Quant Time: Jul 18 02:07:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071520.M
Quant Title :
QLast Update : Thu Jul 16 02:29:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

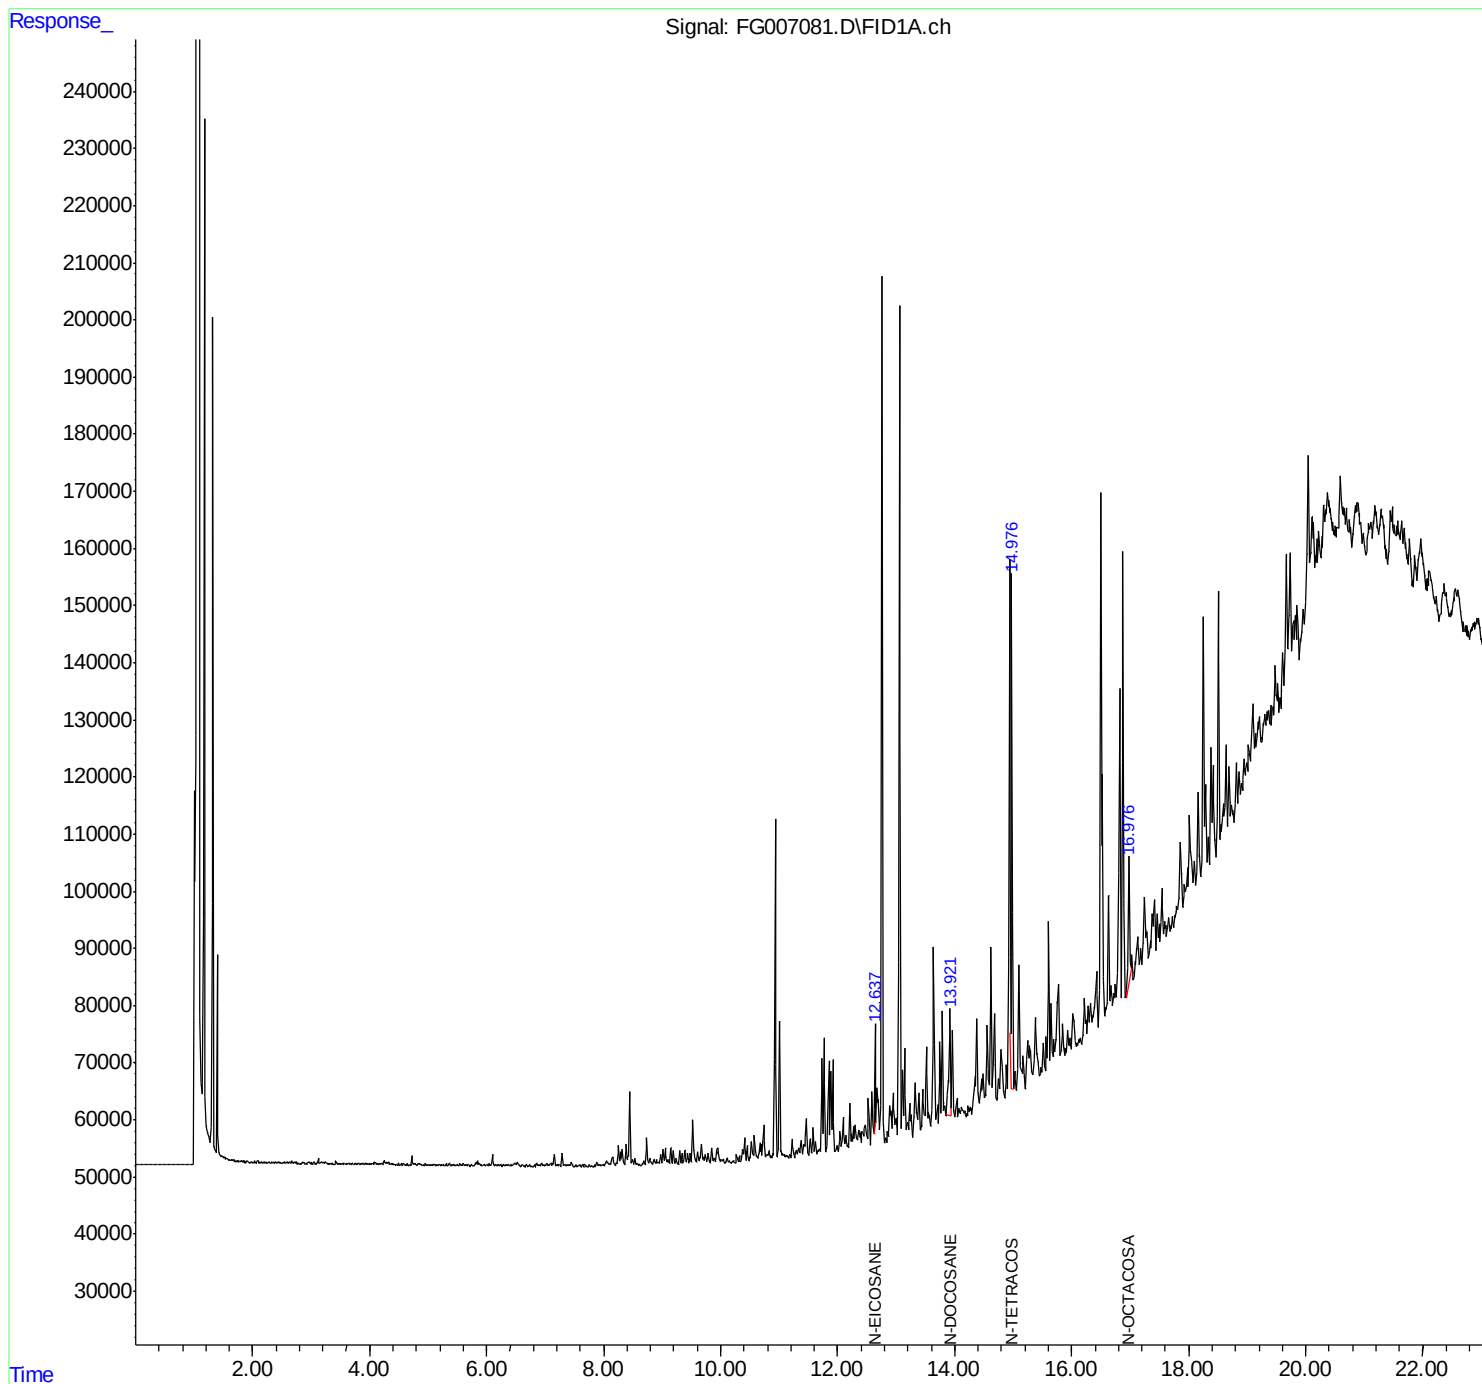


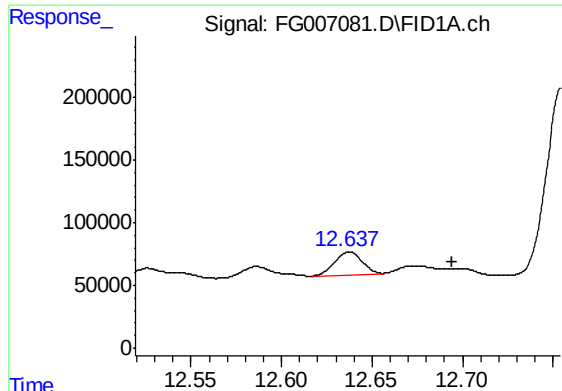

#7 N-EICOSANE


R.T.: 12.637 min
Delta R.T.: -0.057 min
Response: 187764
Conc: 1.01 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-03-071520

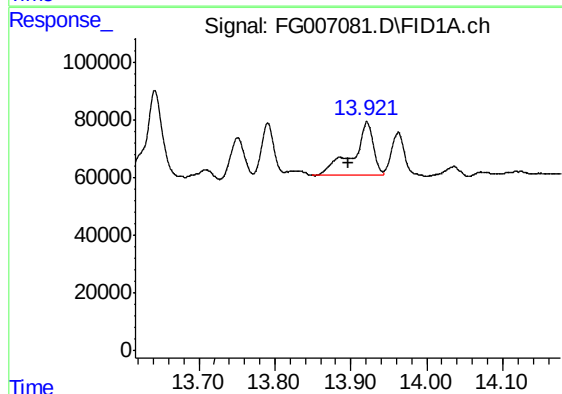


#8 N-DOCOSANE

R.T.: 13.921 min
Delta R.T.: 0.025 min
Response: 351270
Conc: 1.89 ug/ml

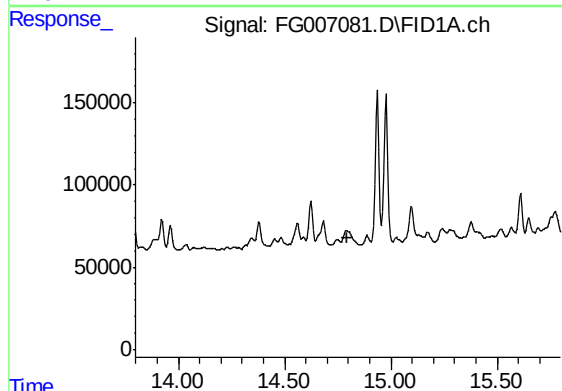


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.798 min
Response: 0
Conc: N.D.

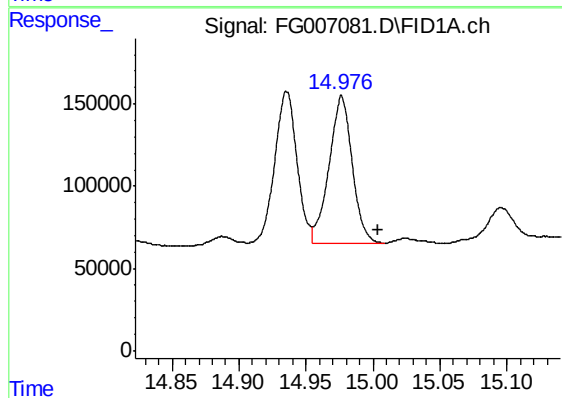

#10 N-TETRACOSANE

R.T.: 14.977 min
Delta R.T.: -0.027 min
Response: 1074139
Conc: 5.75 ug/ml

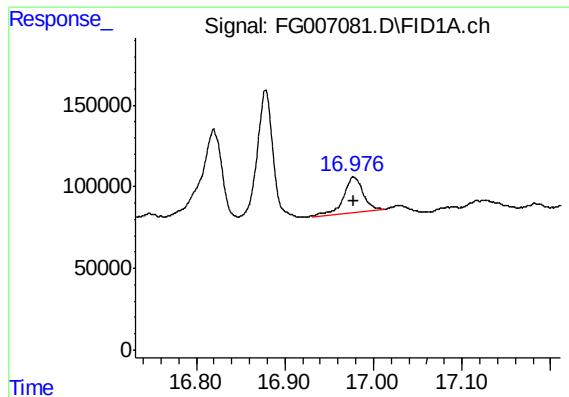

#12 N-OCTACOSANE

R.T.: 16.978 min
Delta R.T.: 0.000 min
Response: 339512
Conc: 1.84 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-03-071520