

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071720\
Data File : FG007076.D
Signal(s) : FID1A.ch
Acq On : 17 Jul 2020 12:57
Operator : DD\AJ
Sample : L3183-11 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-03-071520

Integration File: autoint1.e
Quant Time: Jul 18 02:06:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071520.M
Quant Title :
QLast Update : Thu Jul 16 02:29:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.787	623827	3.816 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071720\
Data File : FG007076.D
Signal(s) : FID1A.ch
Acq On : 17 Jul 2020 12:57
Operator : DD\AJ
Sample : L3183-11 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-03-071520

Integration File: autoint1.e
Quant Time: Jul 18 02:06:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071520.M
Quant Title :
QLast Update : Thu Jul 16 02:29:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

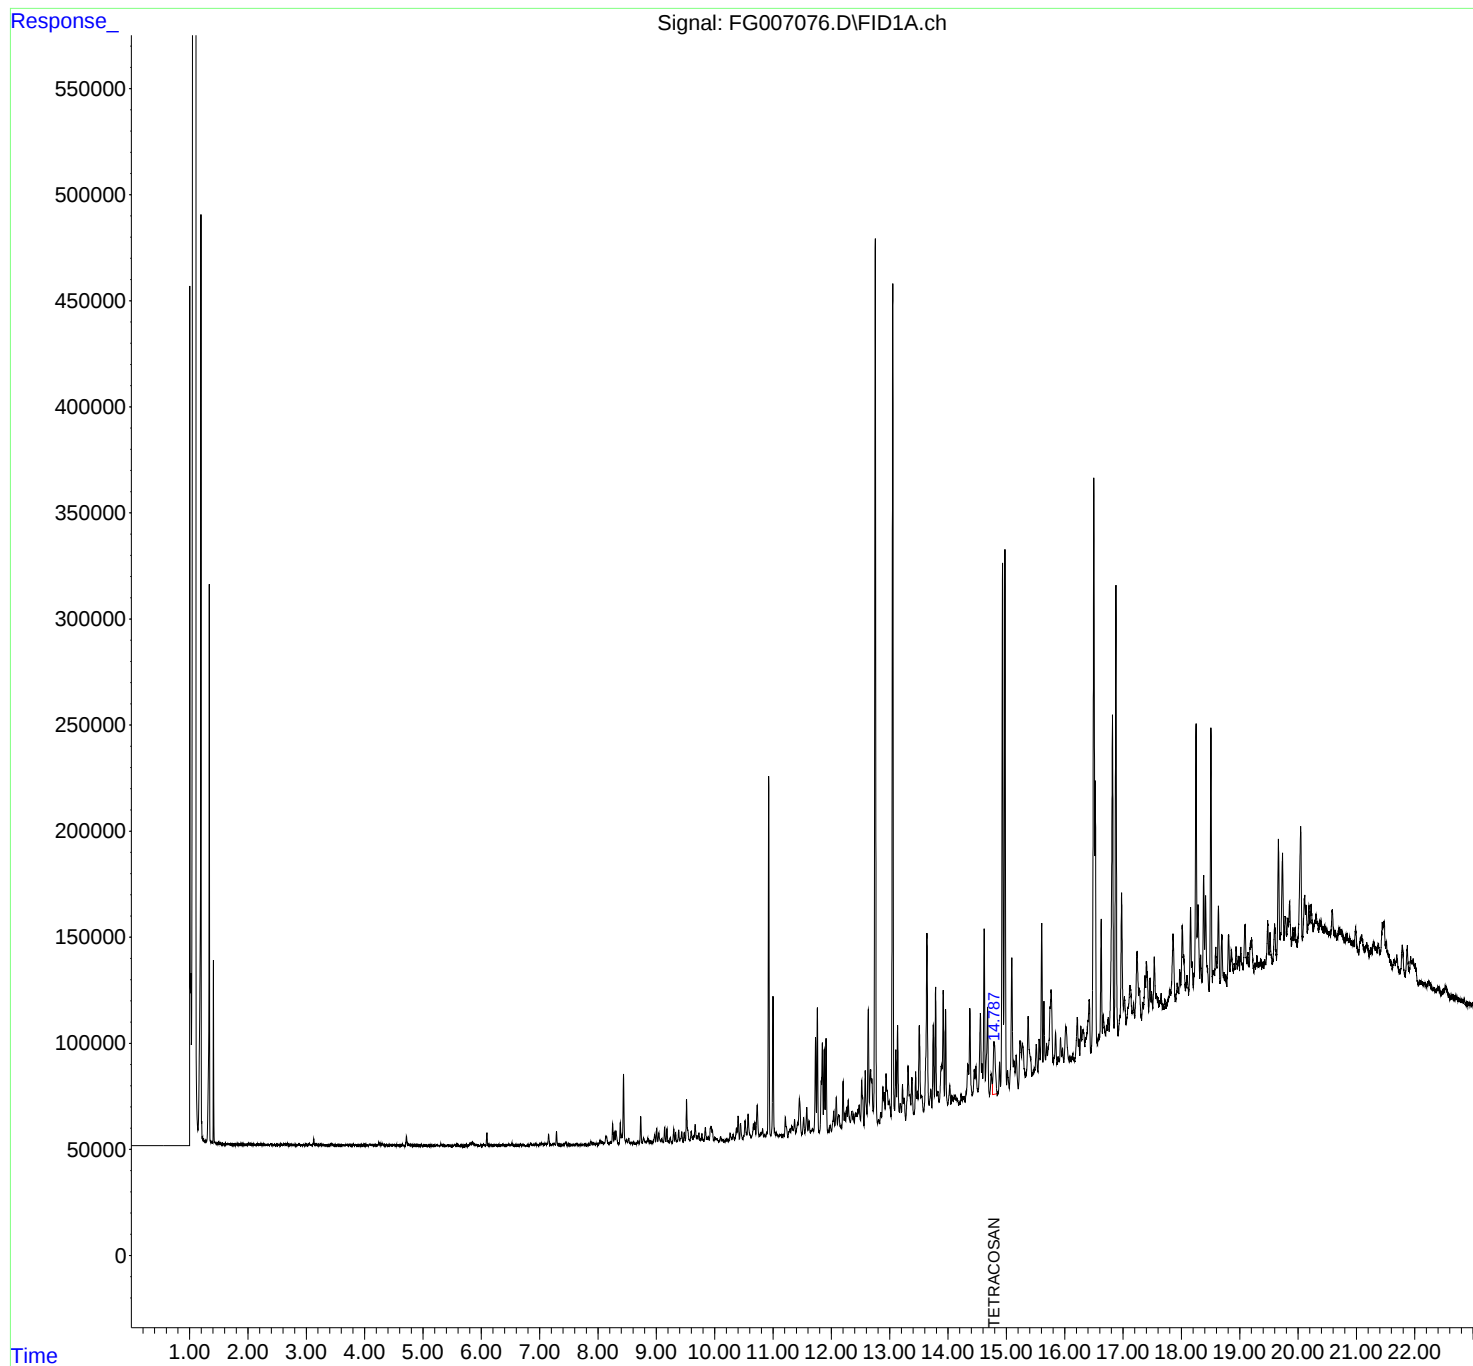

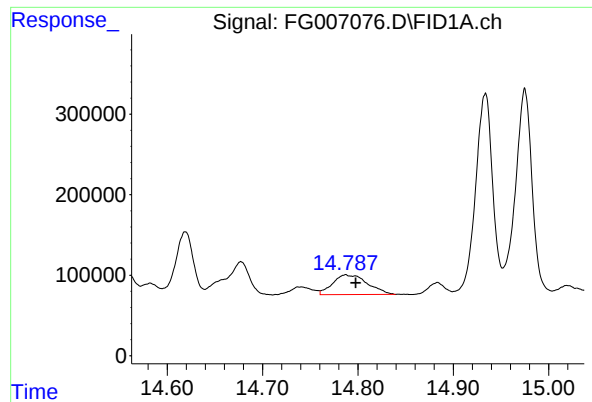

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.787 min
Delta R.T.: -0.011 min
Response: 623827
Conc: 3.82 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-03-071520