

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071721\
 Data File : FG008535.D
 Signal(s) : FID1A.ch
 Acq On : 16 Jul 2021 20:40
 Operator : DD\AJ
 Sample : M2940-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 17 00:31:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.759	2845718	19.971 ug/ml
Target Compounds			
2) N-DECANE	4.463	346573	2.301 ug/ml
3) N-DODECANE	6.489	378293	2.458 ug/ml
4) N-TETRADECANE	8.291	370426	2.378 ug/ml
5) N-HEXADECANE	9.897	365599	2.355 ug/ml
6) N-OCTADECANE	11.342	391393	2.421 ug/ml
7) N-EICOSANE	12.655	401579	2.464 ug/ml
8) N-DOCOSANE	13.855	414043	2.541 ug/ml
10) N-TETRACOSANE	14.963	419122	2.556 ug/ml
11) N-HEXACOSANE	15.987	412581	2.544 ug/ml
12) N-OCTACOSANE	16.937	441584	2.756 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071721\
Data File : FG008535.D
Signal(s) : FID1A.ch
Acq On : 16 Jul 2021 20:40
Operator : DD\AJ
Sample : M2940-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 17 00:31:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

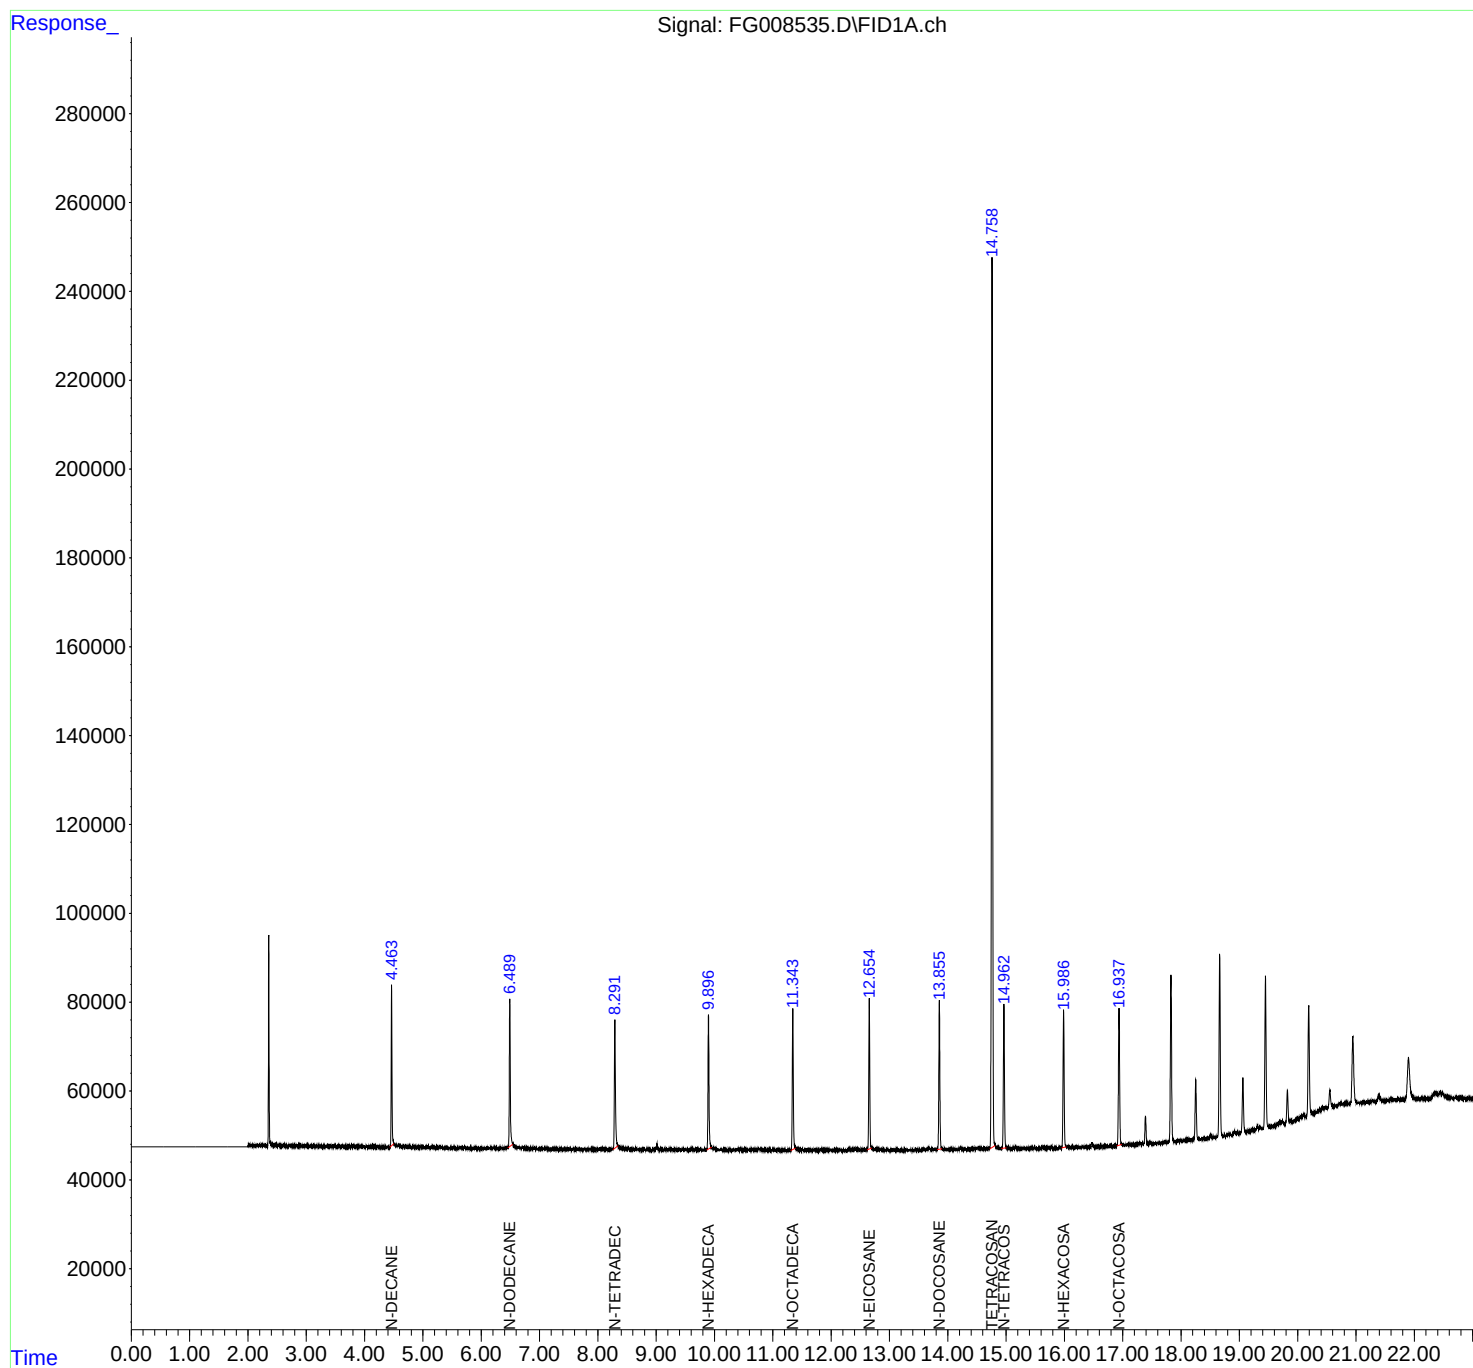

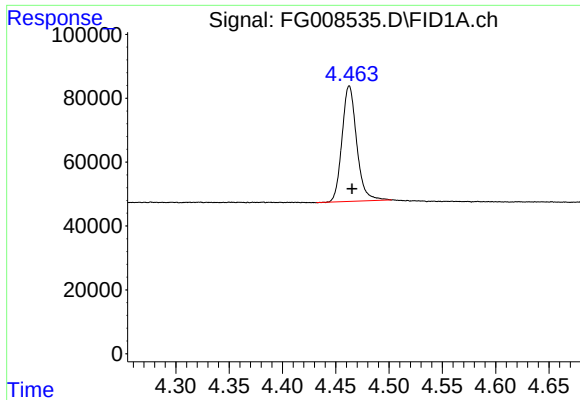


#2 N-DECANE

R.T.: 4.463 min
Delta R.T.: -0.003 min
Response: 346573
Conc: 2.30 ug/ml

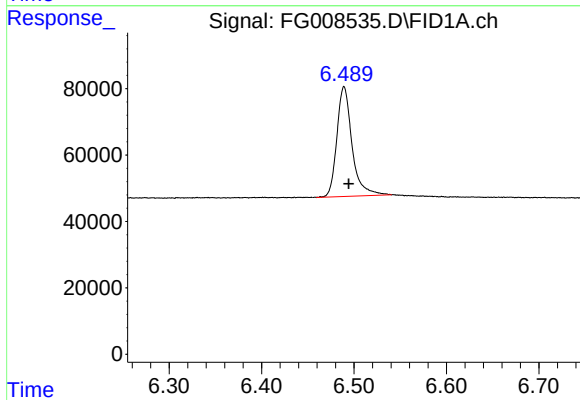


#3 N-DODECANE

R.T.: 6.489 min
Delta R.T.: -0.005 min
Response: 378293
Conc: 2.46 ug/ml

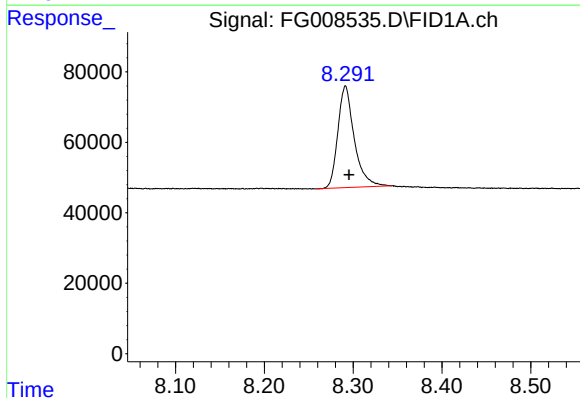


#4 N-TETRADECANE

R.T.: 8.291 min
Delta R.T.: -0.004 min
Response: 370426
Conc: 2.38 ug/ml

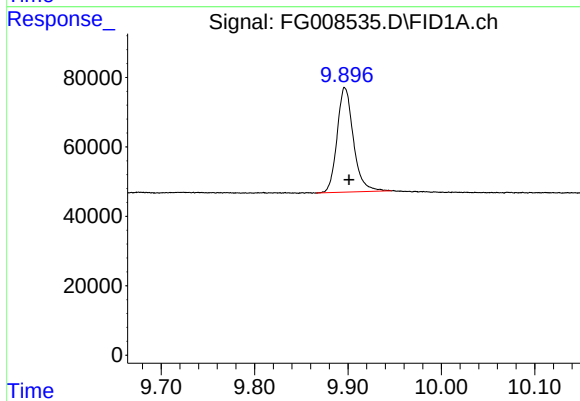


#5 N-HEXADECANE

R.T.: 9.897 min
Delta R.T.: -0.004 min
Response: 365599
Conc: 2.35 ug/ml

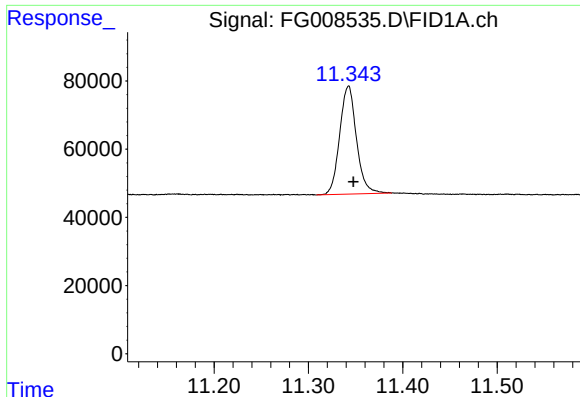


#6 N-OCTADECANE

R.T.: 11.342 min
Delta R.T.: -0.005 min
Response: 391393
Conc: 2.42 ug/ml

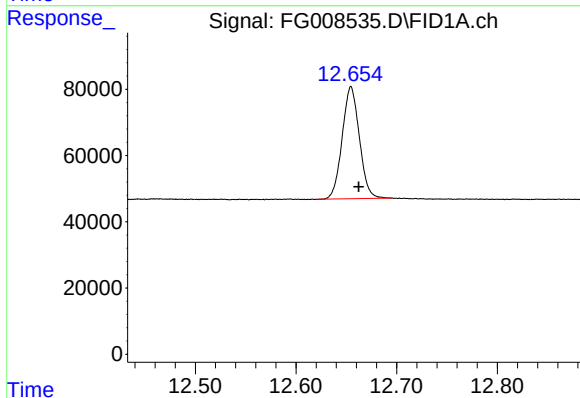


#7 N-EICOSANE

R.T.: 12.655 min
Delta R.T.: -0.008 min
Response: 401579
Conc: 2.46 ug/ml

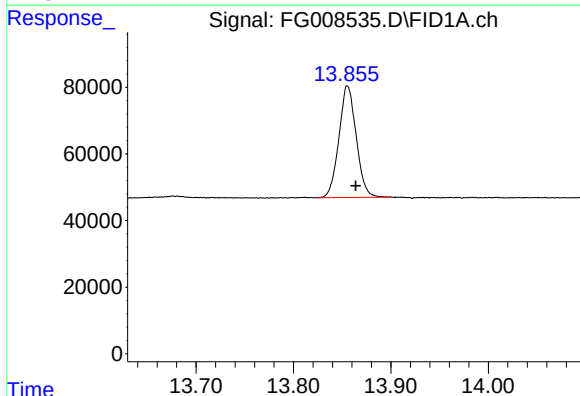


#8 N-DOCOSANE

R.T.: 13.855 min
Delta R.T.: -0.008 min
Response: 414043
Conc: 2.54 ug/ml

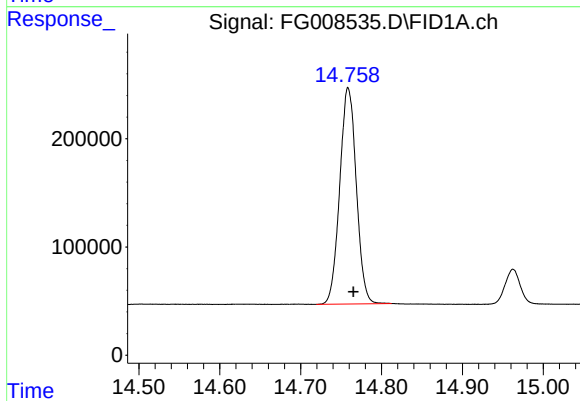


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.759 min
Delta R.T.: -0.007 min
Response: 2845718
Conc: 19.97 ug/ml

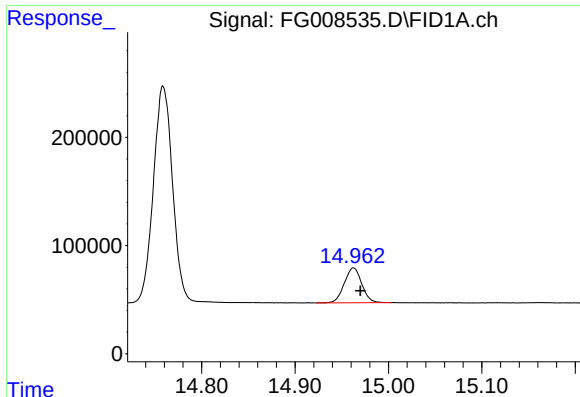


#10 N-TETRACOSANE

R.T.: 14.963 min
Delta R.T.: -0.007 min
Response: 419122
Conc: 2.56 ug/ml

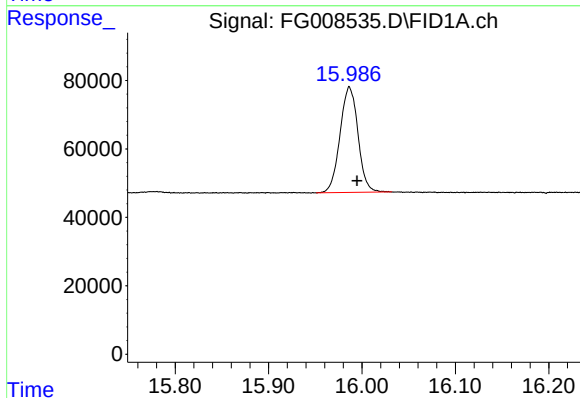

#11 N-HEXACOSANE

R.T.: 15.987 min
Delta R.T.: -0.008 min
Response: 412581
Conc: 2.54 ug/ml

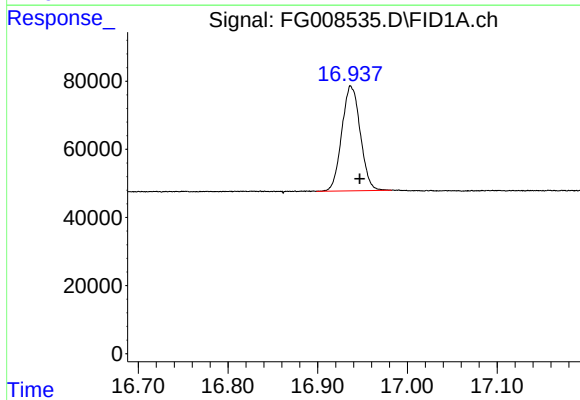

#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: -0.010 min
Response: 441584
Conc: 2.76 ug/ml