

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071721\
 Data File : FG008537.D
 Signal(s) : FID1A.ch
 Acq On : 16 Jul 2021 21:43
 Operator : DD\AJ
 Sample : M2940-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 17 00:31:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
 Quant Title :
 QLast Update : Thu Jul 15 13:17:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.757	2984137	20.943 ug/ml
Target Compounds				
2)	N-DECANE	4.462	740505	4.916 ug/ml
3)	N-DODECANE	6.488	782203	5.083 ug/ml
4)	N-TETRADECANE	8.290	783545	5.029 ug/ml
5)	N-HEXADECANE	9.895	771758	4.971 ug/ml
6)	N-OCTADECANE	11.340	807723	4.996 ug/ml
7)	N-EICOSANE	12.654	825902	5.068 ug/ml
8)	N-DOCOSANE	13.854	836302	5.132 ug/ml
10)	N-TETRACOSANE	14.961	841478	5.131 ug/ml
11)	N-HEXACOSANE	15.985	824656	5.086 ug/ml
12)	N-OCTACOSANE	16.937	830327	5.181 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071721\
Data File : FG008537.D
Signal(s) : FID1A.ch
Acq On : 16 Jul 2021 21:43
Operator : DD\AJ
Sample : M2940-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 17 00:31:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071521.M
Quant Title :
QLast Update : Thu Jul 15 13:17:03 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

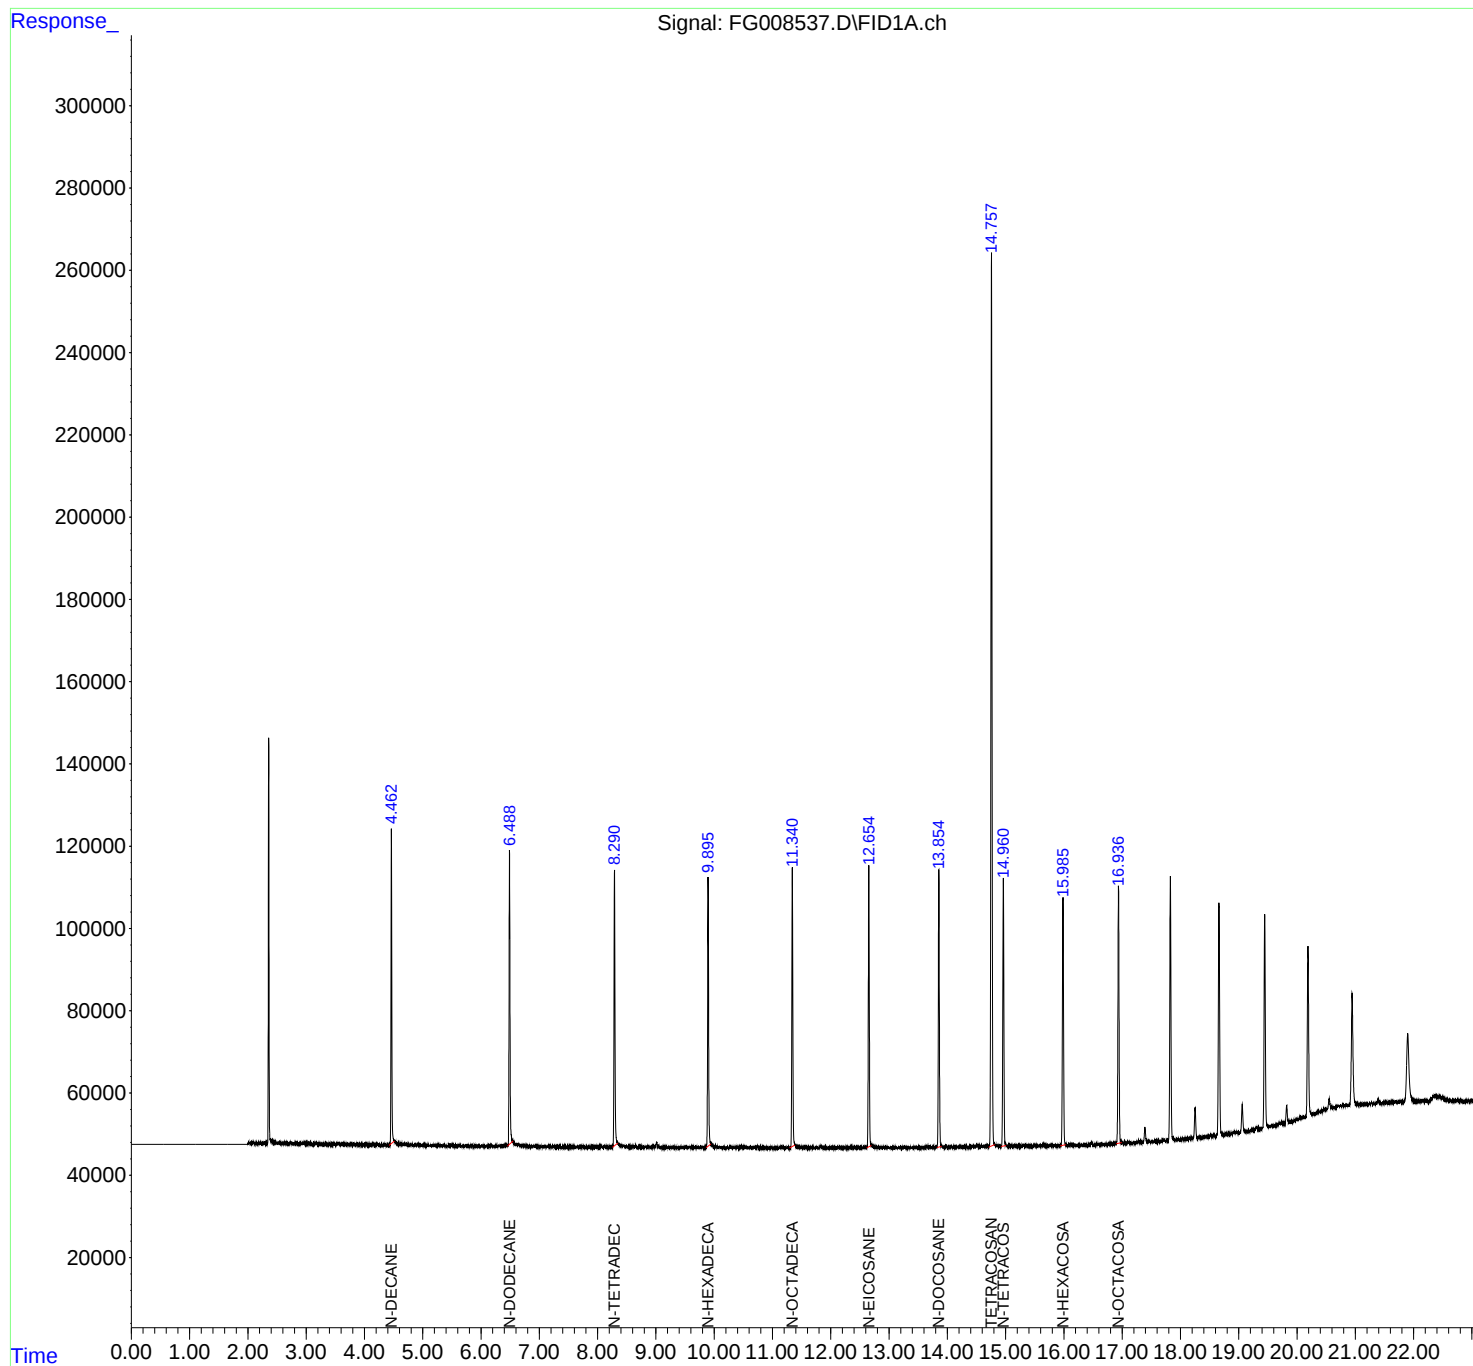

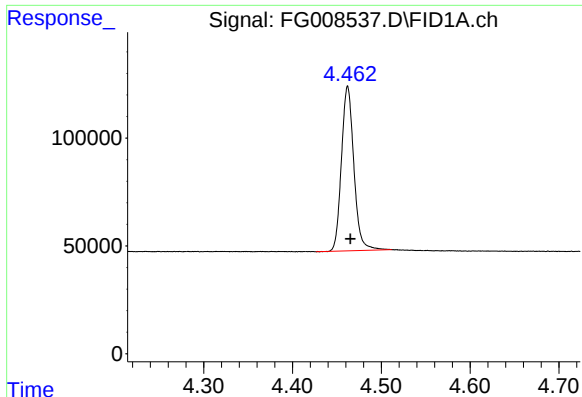


#2 N-DECANE

R.T.: 4.462 min
Delta R.T.: -0.003 min
Response: 740505
Conc: 4.92 ug/ml

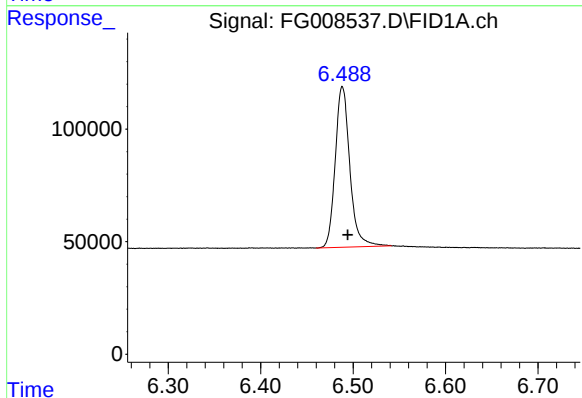


#3 N-DODECANE

R.T.: 6.488 min
Delta R.T.: -0.006 min
Response: 782203
Conc: 5.08 ug/ml

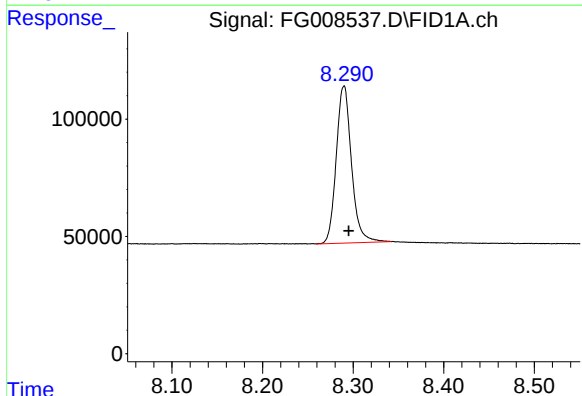


#4 N-TETRADECANE

R.T.: 8.290 min
Delta R.T.: -0.005 min
Response: 783545
Conc: 5.03 ug/ml

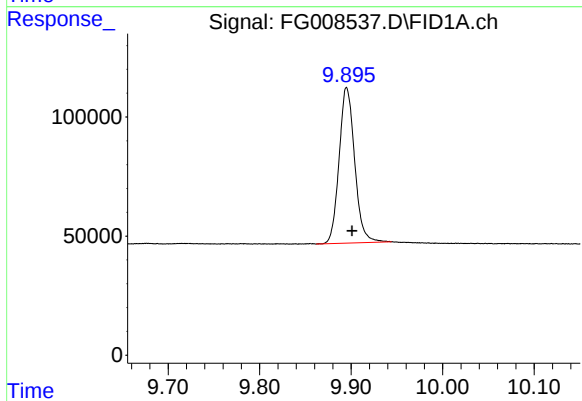


#5 N-HEXADECANE

R.T.: 9.895 min
Delta R.T.: -0.006 min
Response: 771758
Conc: 4.97 ug/ml

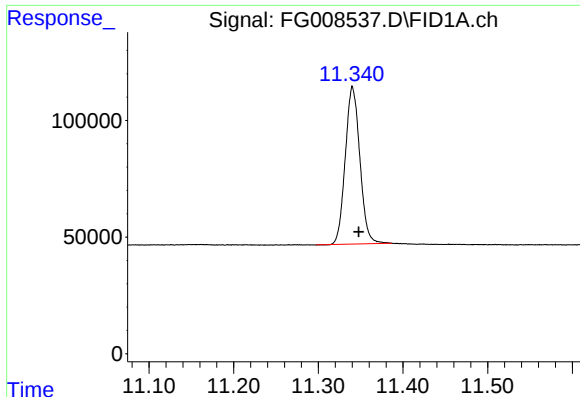


#6 N-OCTADECANE

R.T.: 11.340 min
Delta R.T.: -0.007 min
Response: 807723
Conc: 5.00 ug/ml

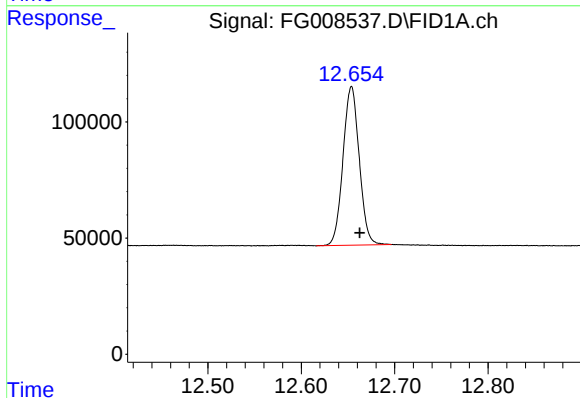


#7 N-EICOSANE

R.T.: 12.654 min
Delta R.T.: -0.009 min
Response: 825902
Conc: 5.07 ug/ml

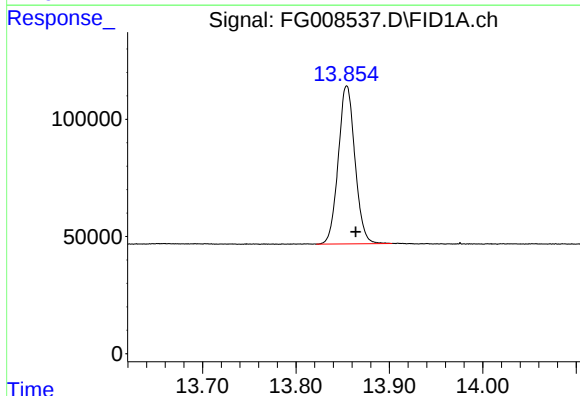


#8 N-DOCOSANE

R.T.: 13.854 min
Delta R.T.: -0.010 min
Response: 836302
Conc: 5.13 ug/ml

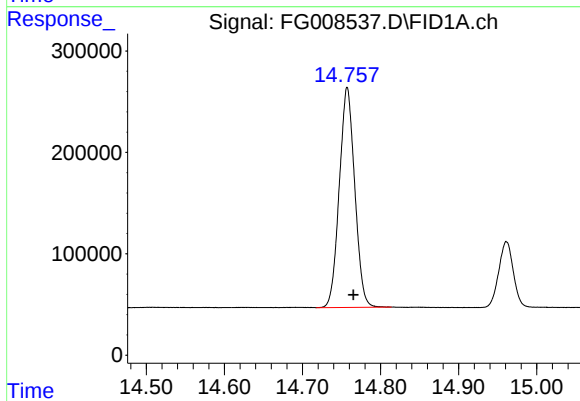


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: -0.008 min
Response: 2984137
Conc: 20.94 ug/ml

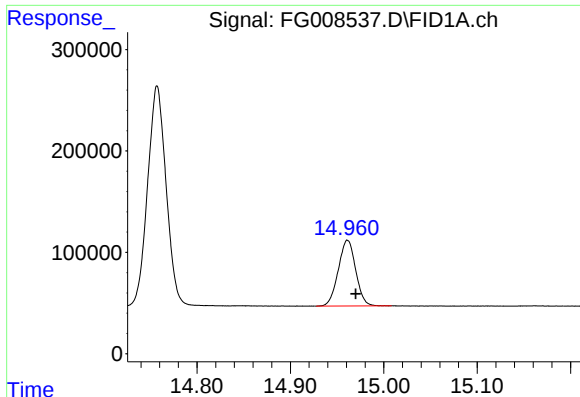


#10 N-TETRACOSANE

R.T.: 14.961 min
Delta R.T.: -0.009 min
Response: 841478
Conc: 5.13 ug/ml

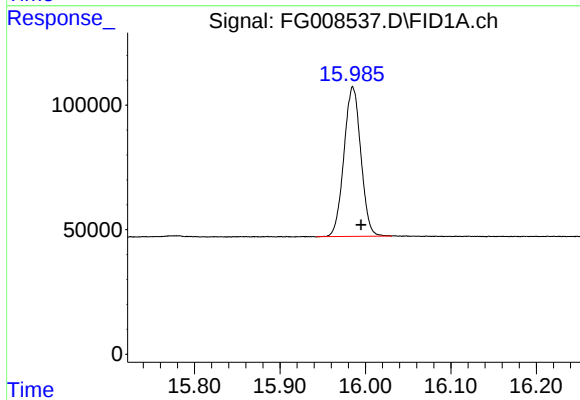

#11 N-HEXACOSANE

R.T.: 15.985 min
Delta R.T.: -0.009 min
Response: 824656
Conc: 5.09 ug/ml

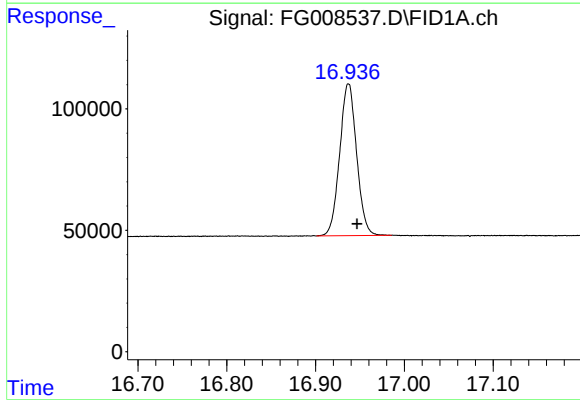

#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: -0.010 min
Response: 830327
Conc: 5.18 ug/ml