

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071723AL\
 Data File : FG012418.D
 Signal(s) : FID1A.ch
 Acq On : 17 Jul 2023 22:23
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 18 05:54:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 01:18:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.162	111602	0.795 ug/ml
18) T n-Dotriacontane (C32)	17.881	28337	0.213 ug/ml
19) T n-Tetratriacontane (C34)	18.664	50981	0.398 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071723AL\
Data File : FG012418.D
Signal(s) : FID1A.ch
Acq On : 17 Jul 2023 22:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 18 05:54:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

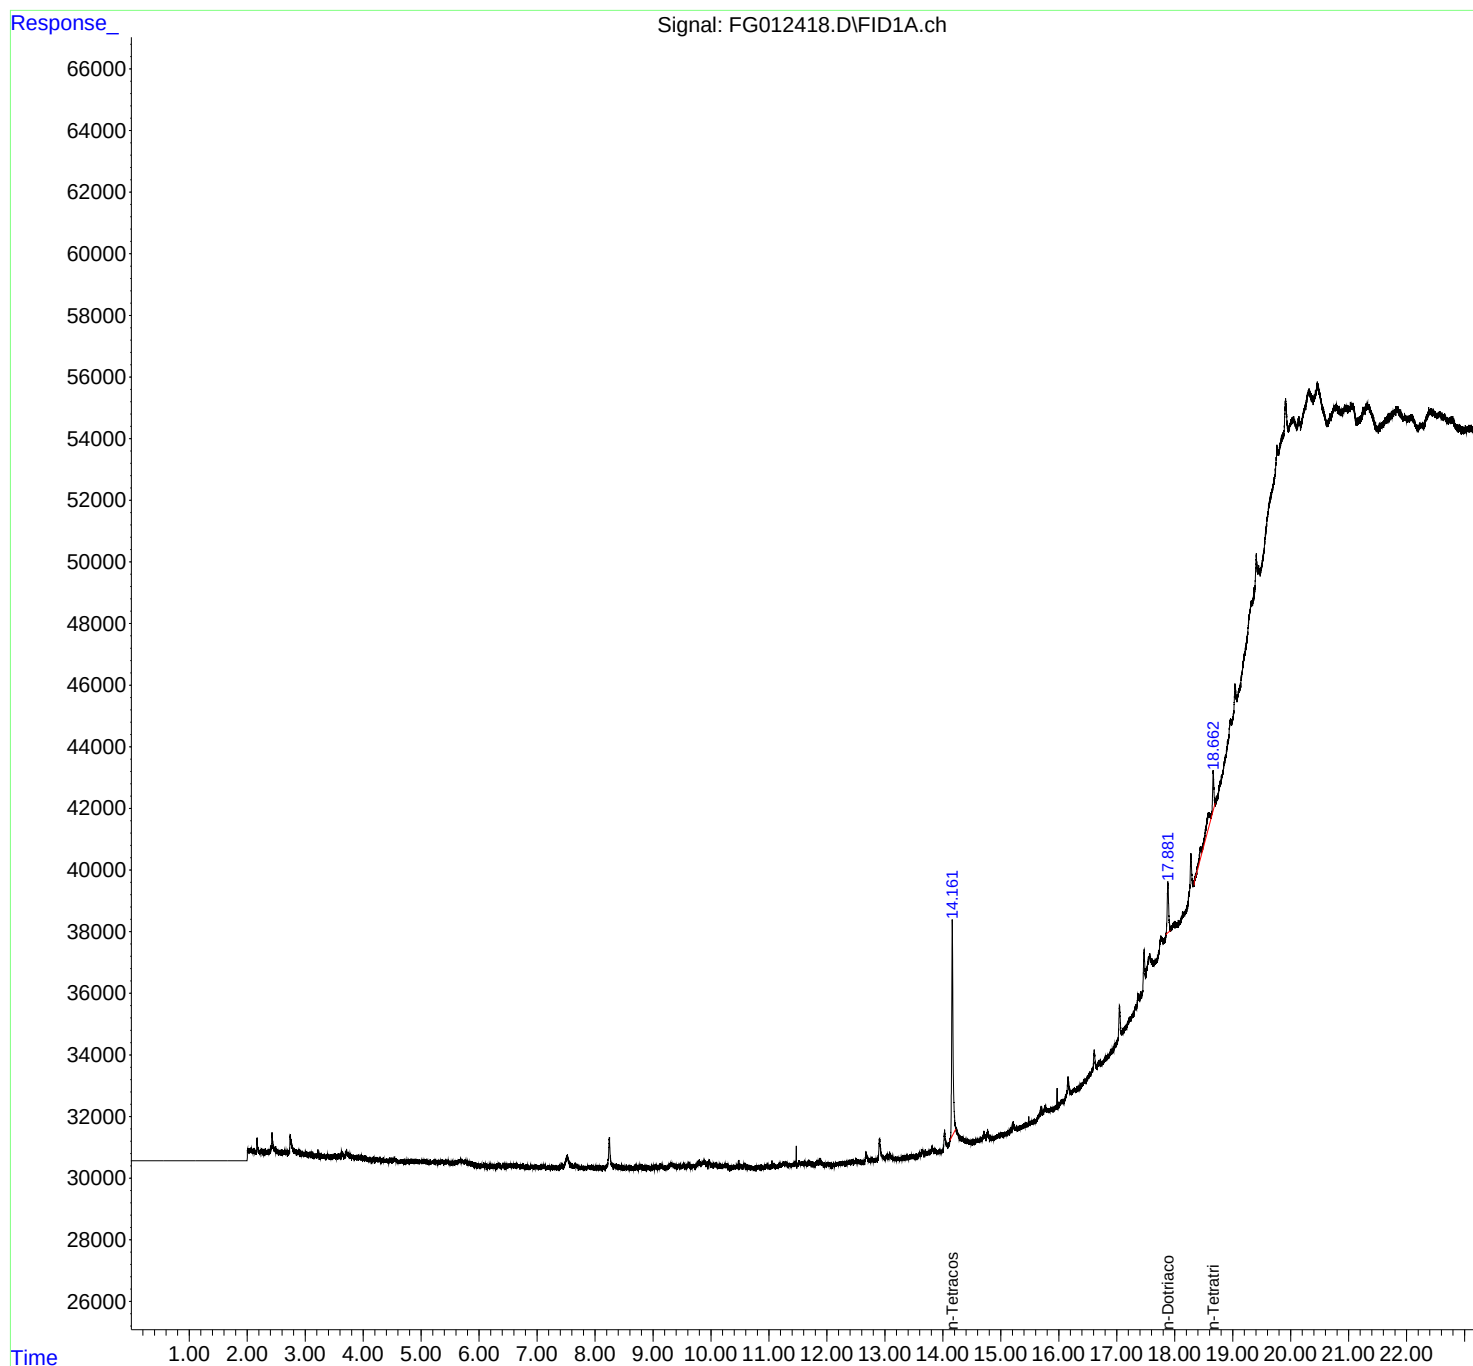

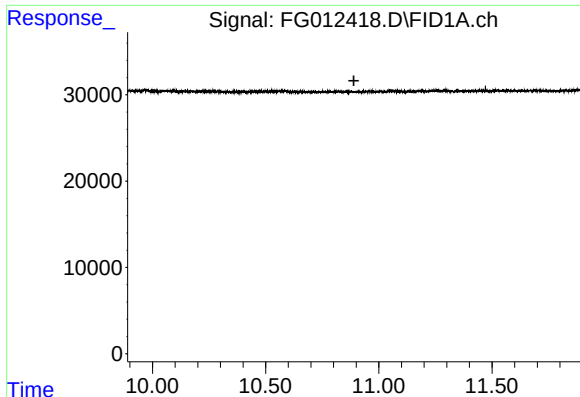


#9 ortho-Terphenyl (SURR)

```

      R.T.:      0.000 min
Exp R.T.  :      10.890 min
  Response:           0
    Conc:      N.D.

```

Instrument :
FID_G
ClientSampleId :

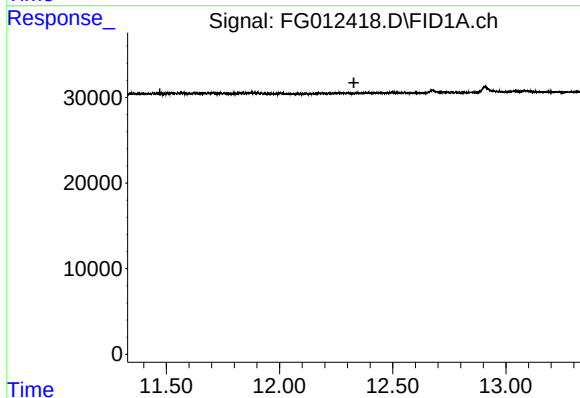


#12 1-chlorooctadecane (SURR)

```

      R.T.:      0.000 min
Exp R.T.  :      12.328 min
Response:         0
      Conc:      N.D.

```

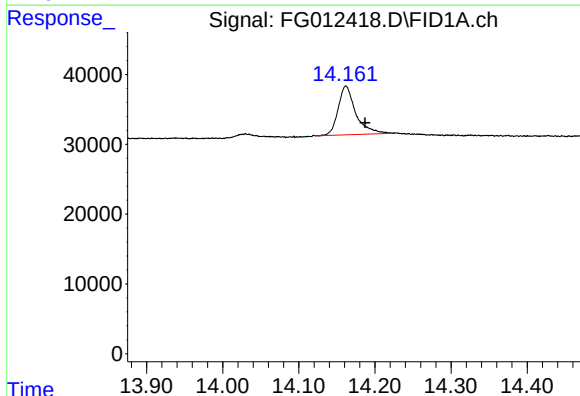


#14 n-Tetracosane (C24)

```

      R.T.:    14.162 min
Delta R.T.:   -0.025 min
  Response:    111602
      Conc:    0.79 ug/ml

```

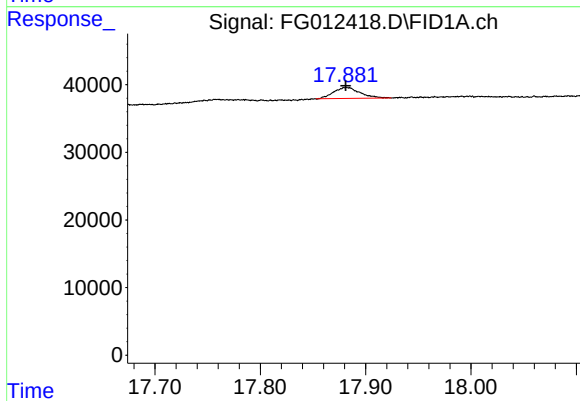


#18 n-Dotriacontane (C32)

```

      R.T.:    17.881 min
Delta R.T.:    0.000 min
  Response:    28337
      Conc:    0.21 ug/ml

```

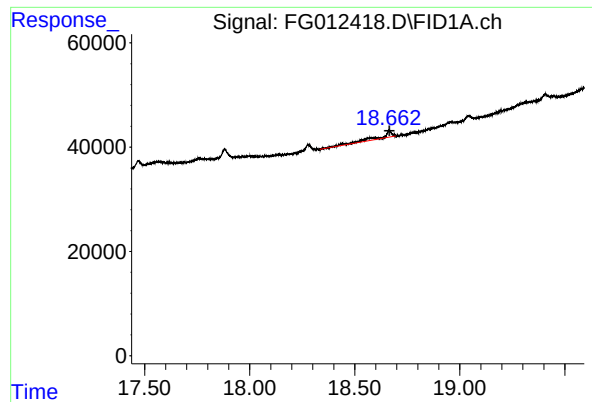

#19 n-Tetratriacontane (C34)

R.T.: 18.664 min
Delta R.T.: -0.001 min
Response: 50981
Conc: 0.40 ug/ml

Instrument :

FID_G

ClientSampleId :