

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071818\
Data File : FG001705.D
Signal(s) : FID1A.ch
Acq On : 18 Jul 2018 15:03
Operator : AJ\SJ
Sample : J4013-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 00:55:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.514	1534725	13.191 ug/ml
Target Compounds			
4) N-TETRADECANE	8.035	523510	3.958 ug/ml
13) N-TRIACONTANE	17.577	175401	1.346 ug/ml
14) N-DOTRIACONTANE	18.410	329419	2.588 ug/ml
16) N-HEXATRIACONTANE	19.942	193621	1.612 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071818\
Data File : FG001705.D
Signal(s) : FID1A.ch
Acq On : 18 Jul 2018 15:03
Operator : AJ\SJ
Sample : J4013-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 00:55:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

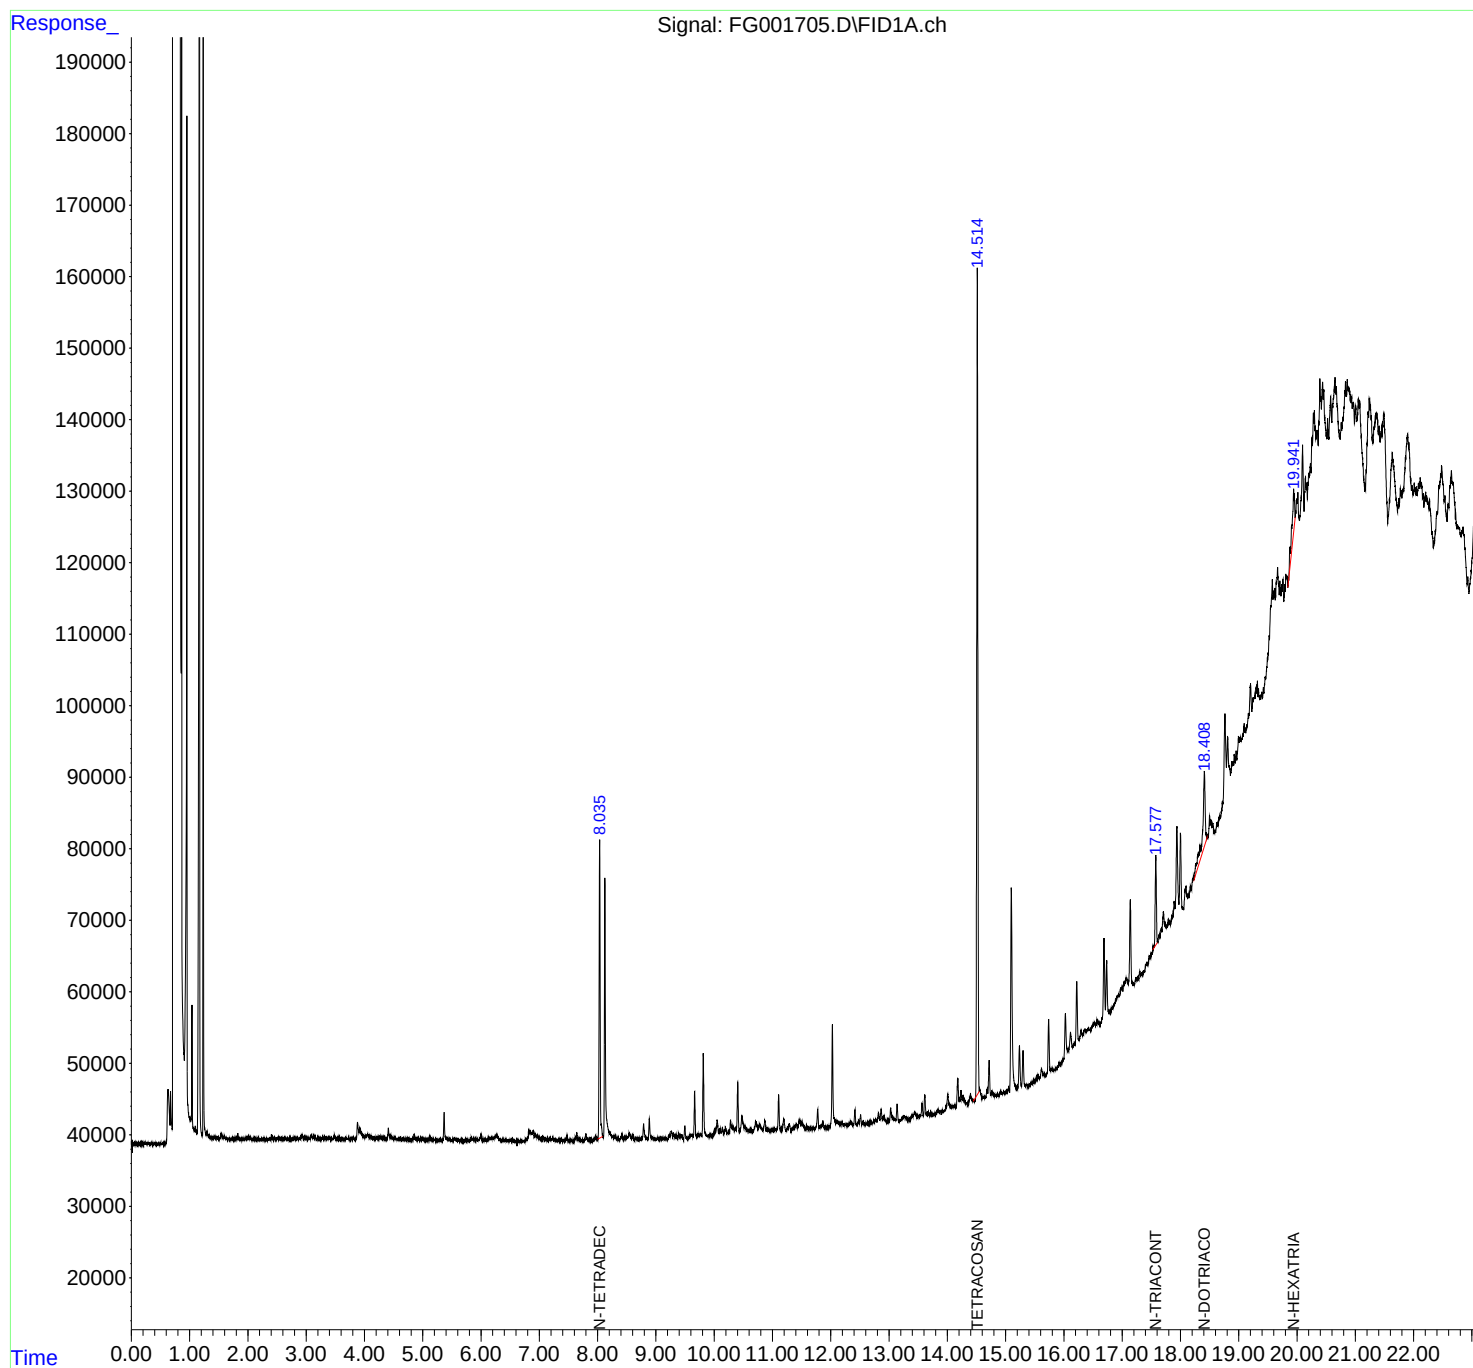

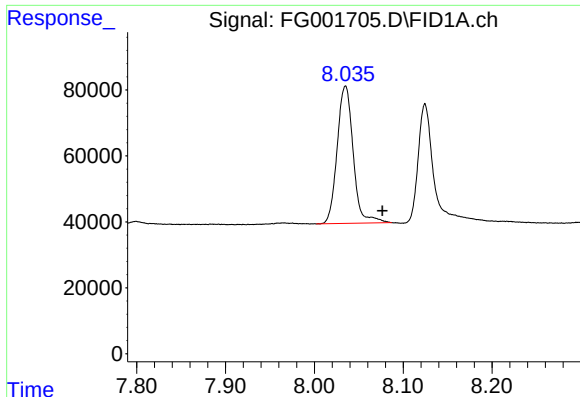


#4 N-TETRADECANE

R.T.: 8.035 min
Delta R.T.: -0.042 min
Response: 523510
Conc: 3.96 ug/ml

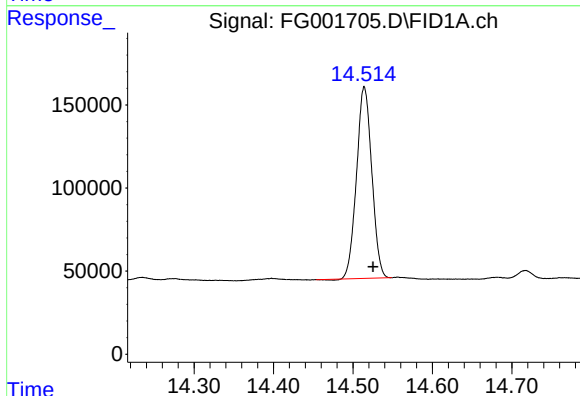


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.514 min
Delta R.T.: -0.011 min
Response: 1534725
Conc: 13.19 ug/ml

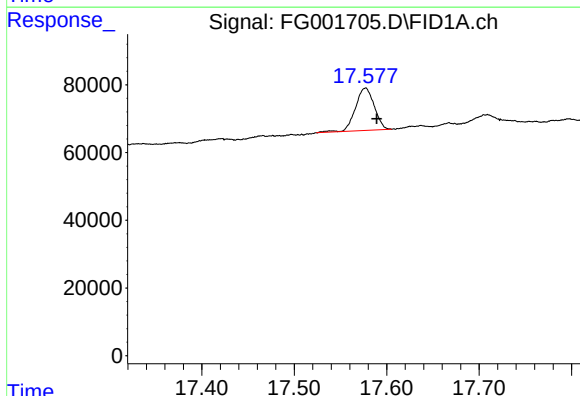


#13 N-TRIACONTANE

R.T.: 17.577 min
Delta R.T.: -0.012 min
Response: 175401
Conc: 1.35 ug/ml

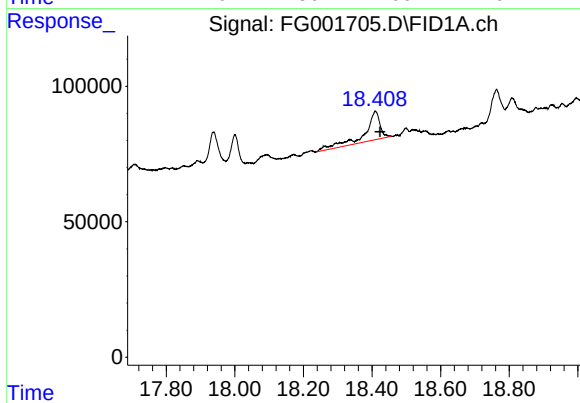

#14 N-DOTRIACONTANE

R.T.: 18.410 min
Delta R.T.: -0.014 min
Response: 329419
Conc: 2.59 ug/ml

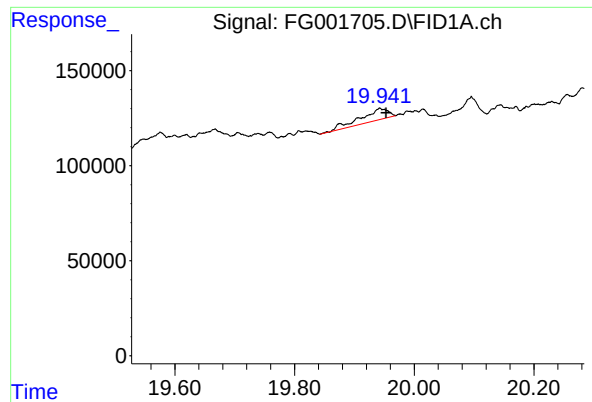

#16 N-HEXATRIACONTANE

R.T.: 19.942 min
Delta R.T.: -0.011 min
Response: 193621
Conc: 1.61 ug/ml