

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071818\
 Data File : FG001715.D
 Signal(s) : FID1A.ch
 Acq On : 18 Jul 2018 20:05
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 19 00:57:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.518	5293190	45.496 ug/ml
Target Compounds			
2) N-DECANE	4.261	6243045	48.390 ug/ml
3) N-DODECANE	6.277	6306936	47.947 ug/ml
4) N-TETRADECANE	8.070	6326035	47.828 ug/ml
5) N-HEXADECANE	9.669	6343739	47.966 ug/ml
6) N-OCTADECANE	11.110	6351177	47.485 ug/ml
7) N-EICOSANE	12.420	6242578	46.766 ug/ml
8) N-DOCOSANE	13.618	6102657	45.862 ug/ml
10) N-TETRACOSANE	14.722	5928182	44.842 ug/ml
11) N-HEXACOSANE	15.743	5780773	43.908 ug/ml
12) N-OCTACOSANE	16.694	5678887	43.439 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071818\
Data File : FG001715.D
Signal(s) : FID1A.ch
Acq On : 18 Jul 2018 20:05
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 19 00:57:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

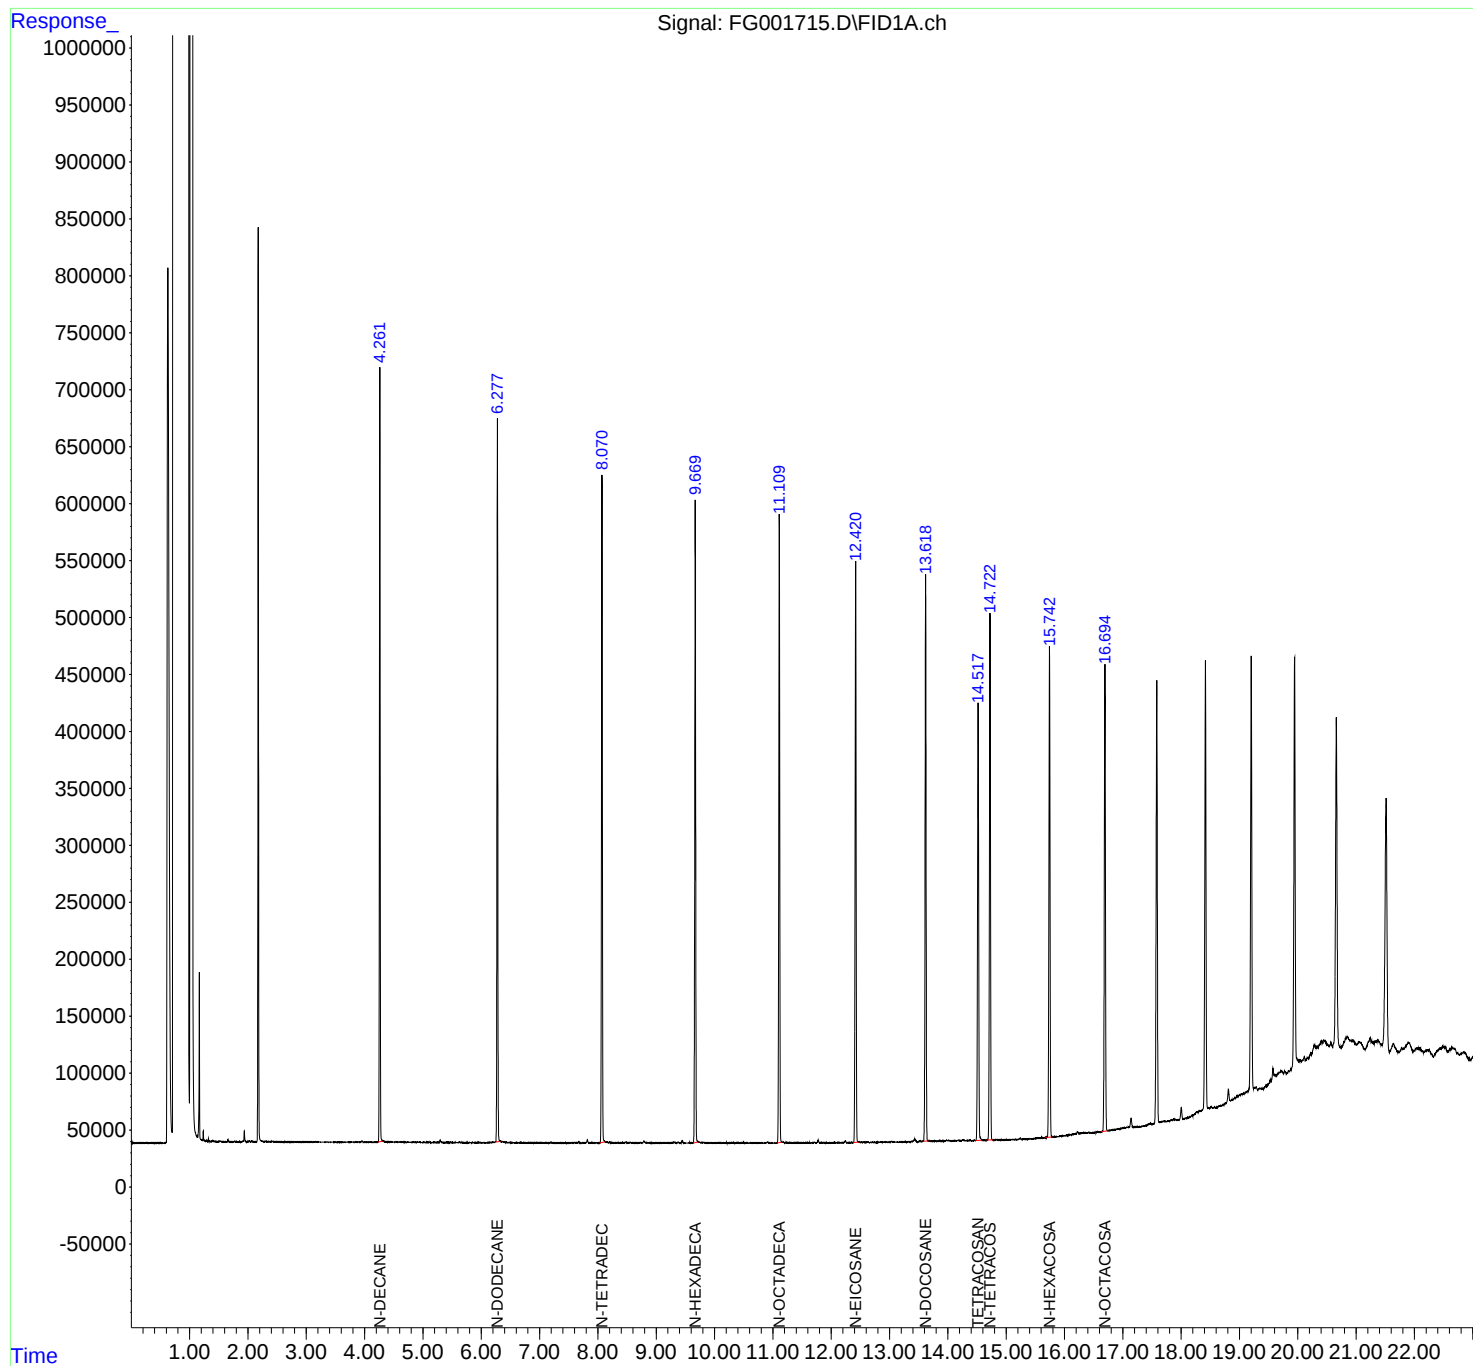

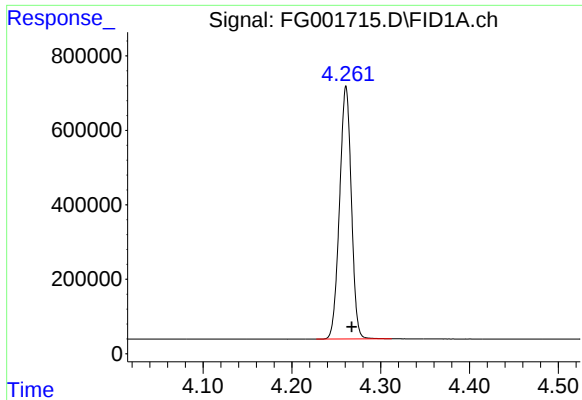


#2 N-DECANE

R.T.: 4.261 min
Delta R.T.: -0.006 min
Response: 6243045
Conc: 48.39 ug/ml

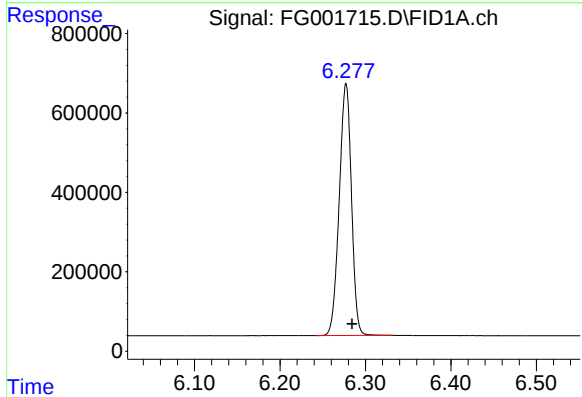


#3 N-DODECANE

R.T.: 6.277 min
Delta R.T.: -0.007 min
Response: 6306936
Conc: 47.95 ug/ml

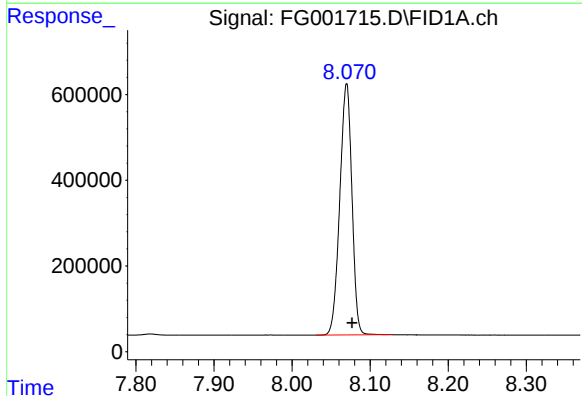


#4 N-TETRADECANE

R.T.: 8.070 min
Delta R.T.: -0.007 min
Response: 6326035
Conc: 47.83 ug/ml

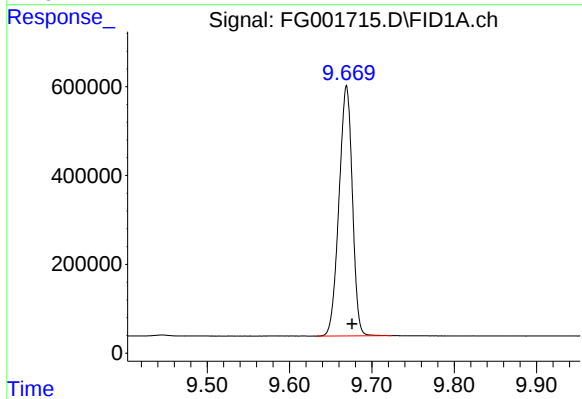


#5 N-HEXADECANE

R.T.: 9.669 min
Delta R.T.: -0.007 min
Response: 6343739
Conc: 47.97 ug/ml

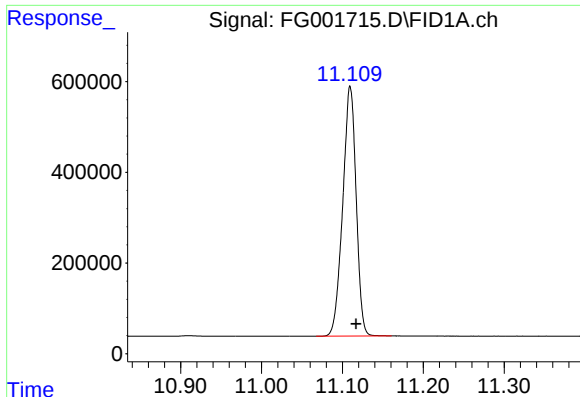


#6 N-OCTADECANE

R.T.: 11.110 min
Delta R.T.: -0.007 min
Response: 6351177
Conc: 47.49 ug/ml

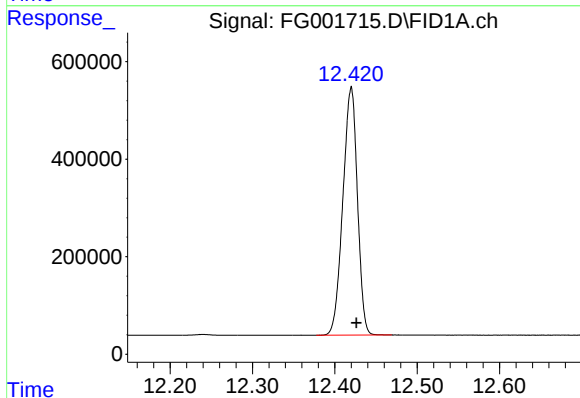


#7 N-EICOSANE

R.T.: 12.420 min
Delta R.T.: -0.006 min
Response: 6242578
Conc: 46.77 ug/ml

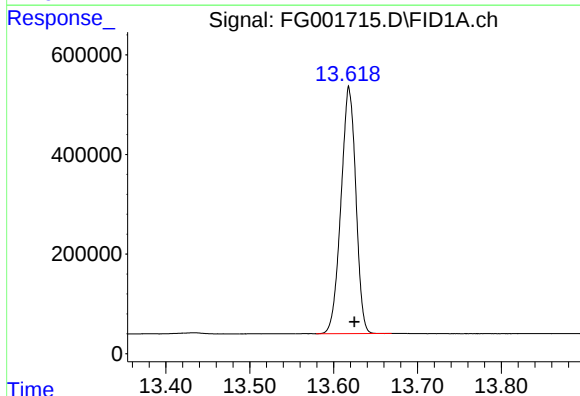


#8 N-DOCOSANE

R.T.: 13.618 min
Delta R.T.: -0.007 min
Response: 6102657
Conc: 45.86 ug/ml

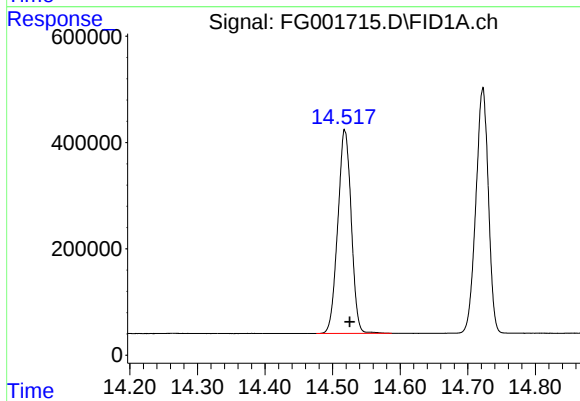


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.518 min
Delta R.T.: -0.007 min
Response: 5293190
Conc: 45.50 ug/ml

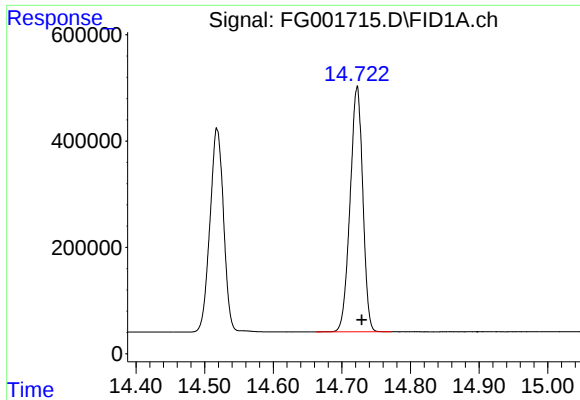


#10 N-TETRACOSANE

R.T.: 14.722 min
Delta R.T.: -0.007 min
Response: 5928182
Conc: 44.84 ug/ml

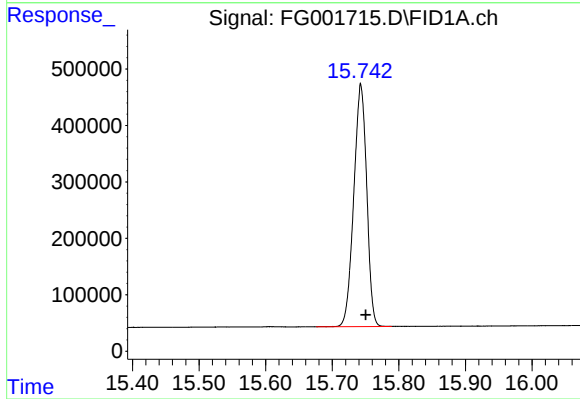

#11 N-HEXACOSANE

R.T.: 15.743 min
Delta R.T.: -0.008 min
Response: 5780773
Conc: 43.91 ug/ml

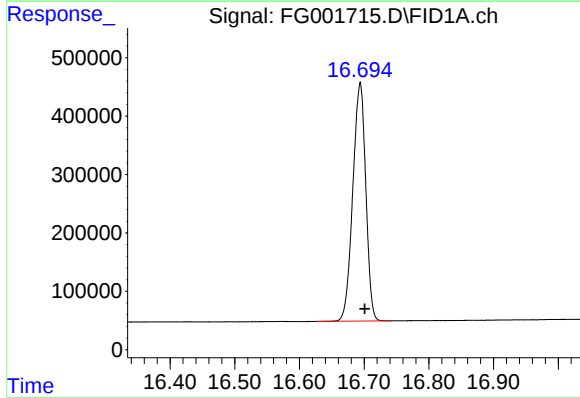

#12 N-OCTACOSANE

R.T.: 16.694 min
Delta R.T.: -0.007 min
Response: 5678887
Conc: 43.44 ug/ml