

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071823AL\
 Data File : FG012423.D
 Signal(s) : FID1A.ch
 Acq On : 18 Jul 2023 08:53
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 19 03:23:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 01:18:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	14.163	275676	1.963 ug/ml
18) T	n-Dotriacontane (C32)	17.884	22294	0.168 ug/ml
19) T	n-Tetratriacontane (C34)	18.666	7669	0.060 ug/ml
22) T	n-Tetracontane (C40)	21.051	21993	0.190 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071823AL\
Data File : FG012423.D
Signal(s) : FID1A.ch
Acq On : 18 Jul 2023 08:53
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 19 03:23:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

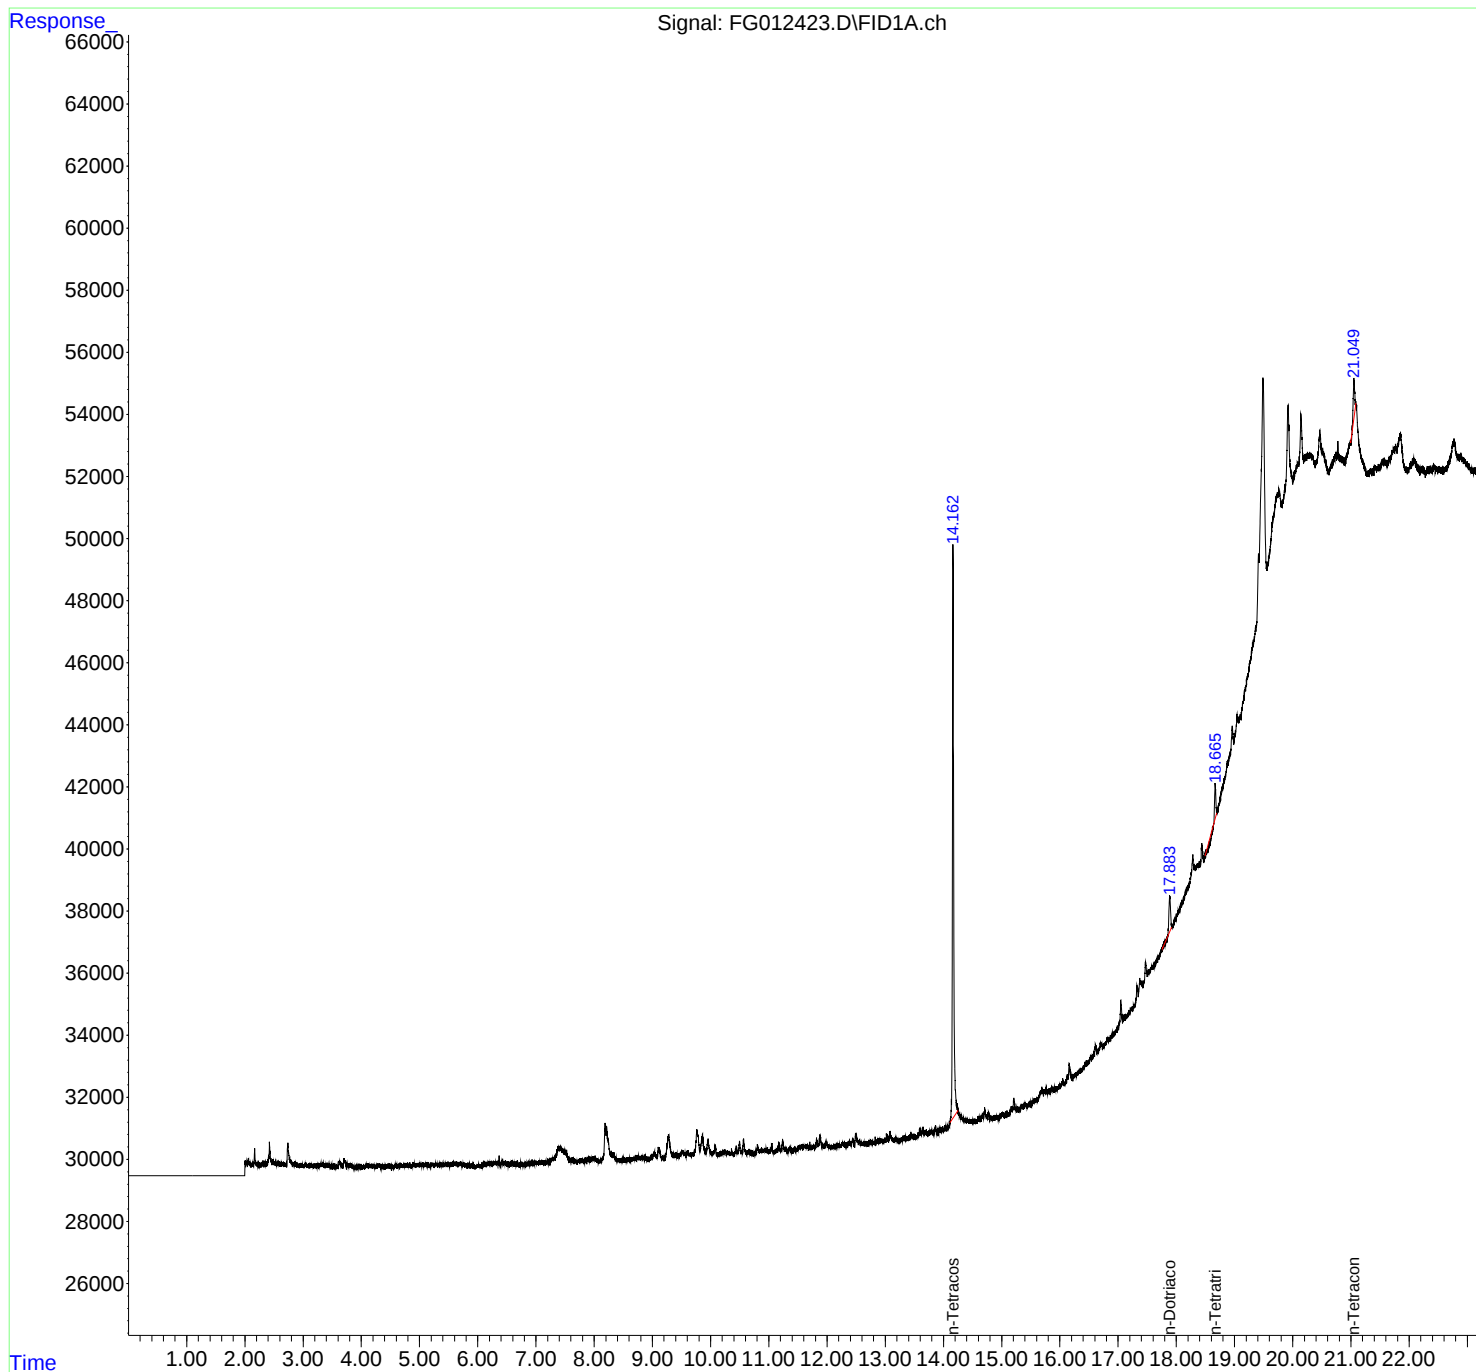


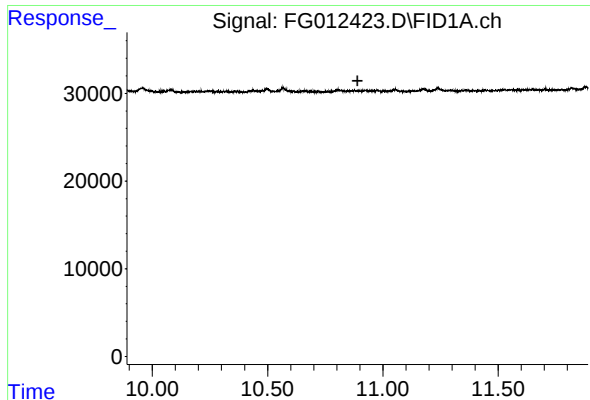

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 10.890 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

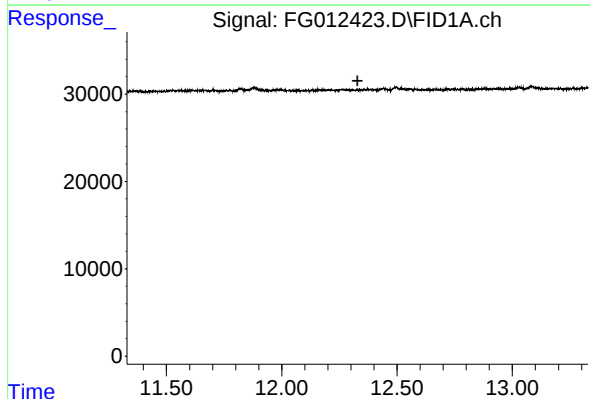


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.328 min
Response: 0
Conc: N.D.

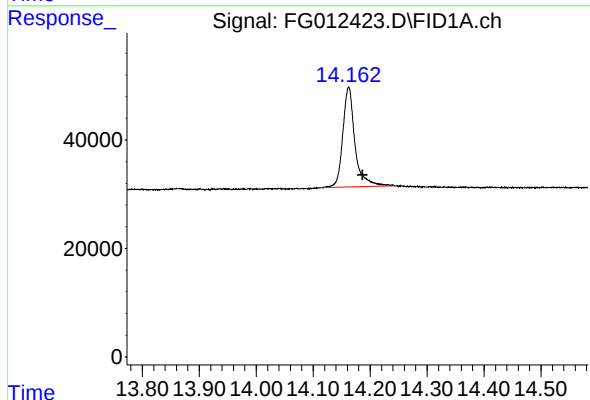


#14 n-Tetracosane (C24)

R.T.: 14.163 min
Delta R.T.: -0.024 min
Response: 275676
Conc: 1.96 ug/ml

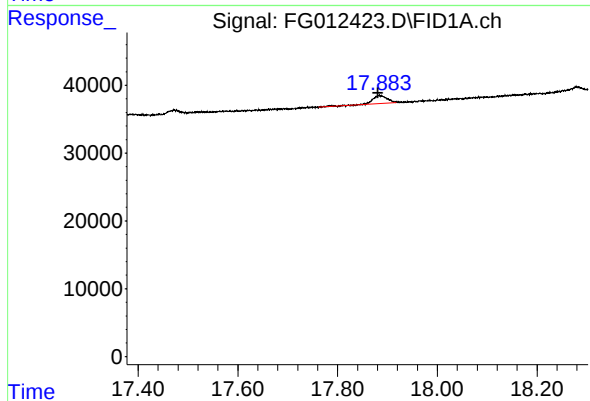

#18 n-Dotriacontane (C32)


R.T.: 17.884 min
Delta R.T.: 0.002 min
Response: 22294
Conc: 0.17 ug/ml

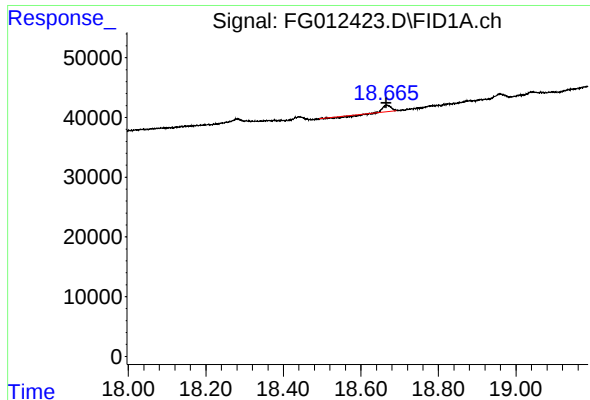

#19 n-Tetratriacontane (C34)

R.T.: 18.666 min
Delta R.T.: 0.001 min
Response: 7669
Conc: 0.06 ug/ml

Instrument :
FID_G
ClientSampleId :

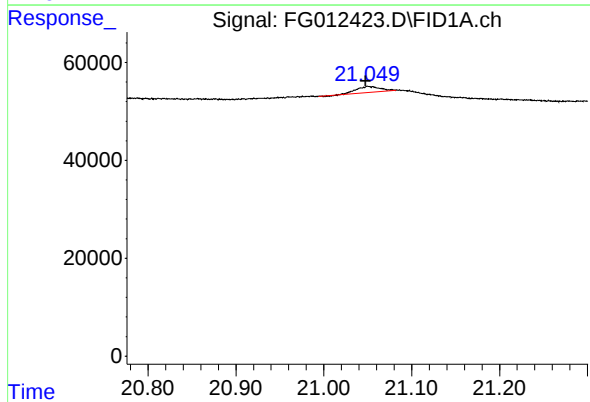

#22 n-Tetracontane (C40)

R.T.: 21.051 min
Delta R.T.: 0.003 min
Response: 21993
Conc: 0.19 ug/ml