

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071823AL\
Data File : FG012438.D
Signal(s) : FID1A.ch
Acq On : 18 Jul 2023 22:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 19 03:25:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	14.159	131621	0.937 ug/ml
18) T	n-Dotriacontane (C32)	17.878	41935	0.315 ug/ml
19) T	n-Tetratriacontane (C34)	18.663	22852	0.178 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071823AL\
Data File : FG012438.D
Signal(s) : FID1A.ch
Acq On : 18 Jul 2023 22:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 19 03:25:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

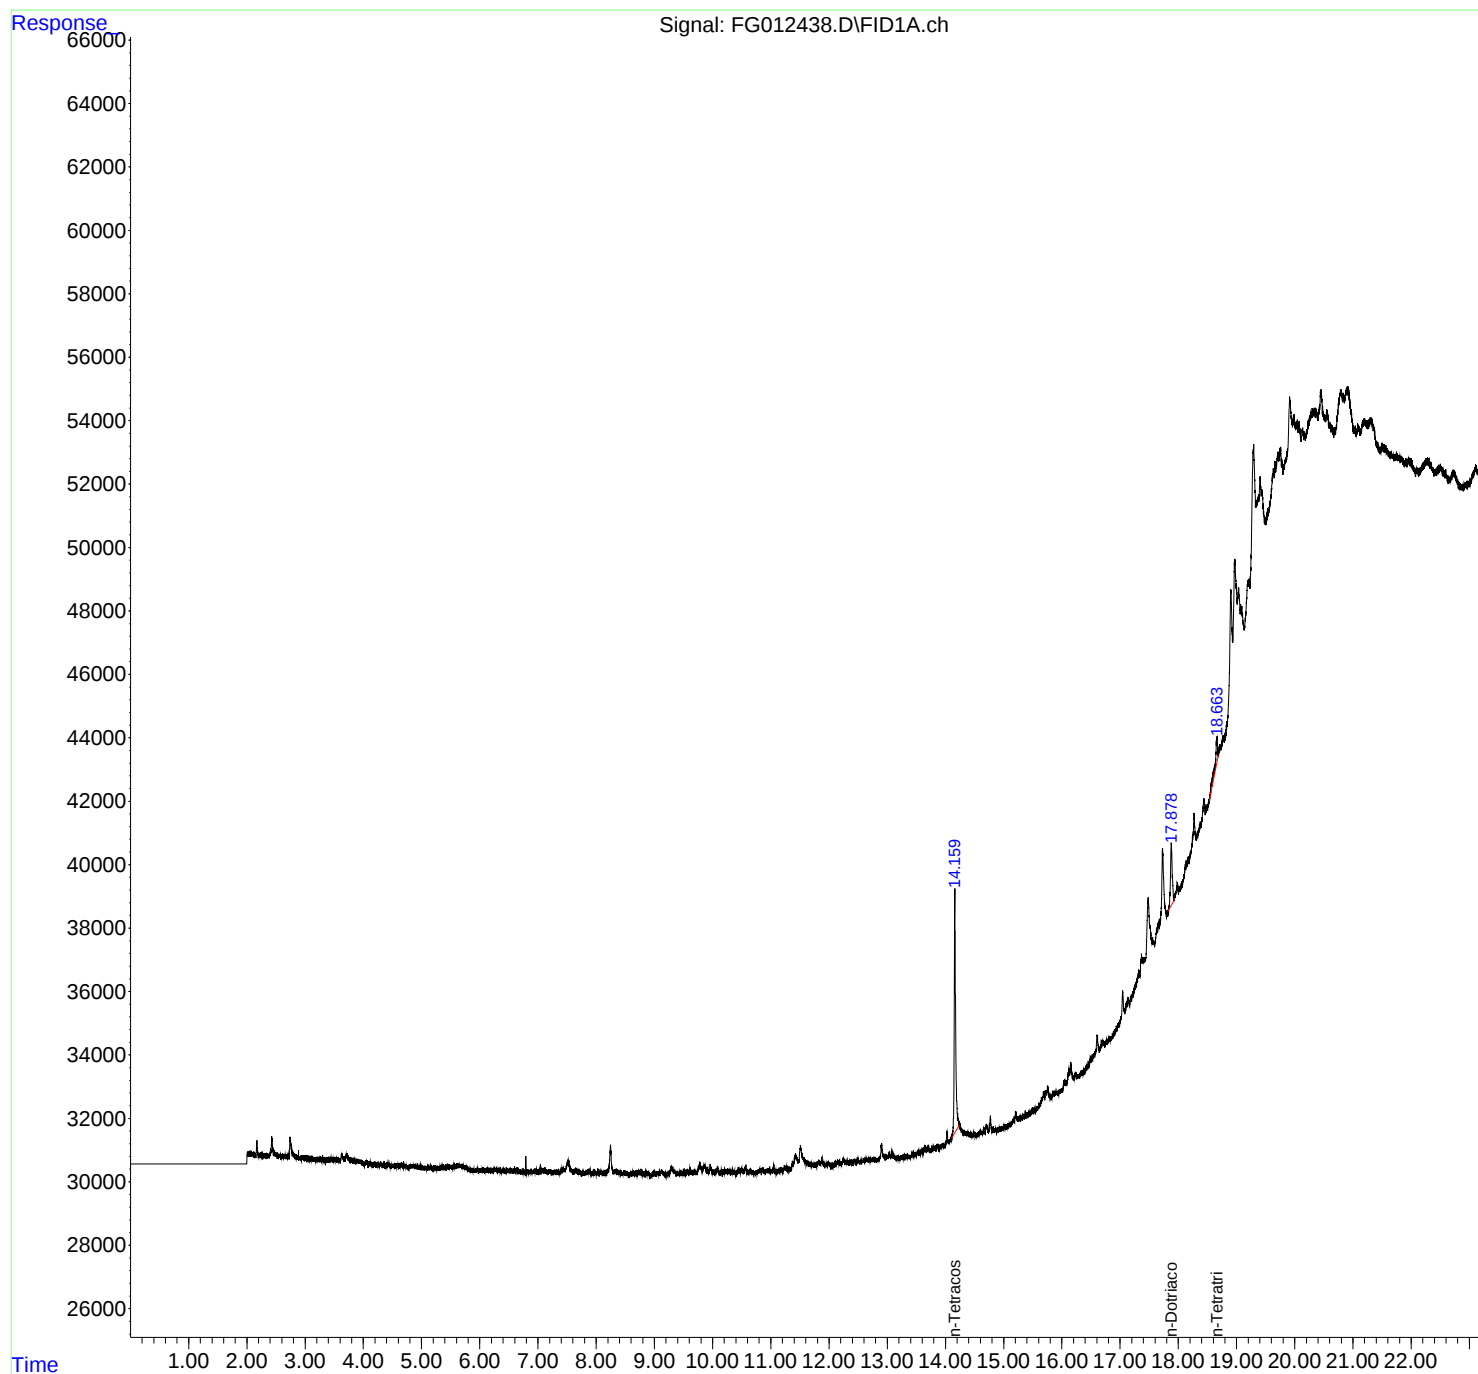


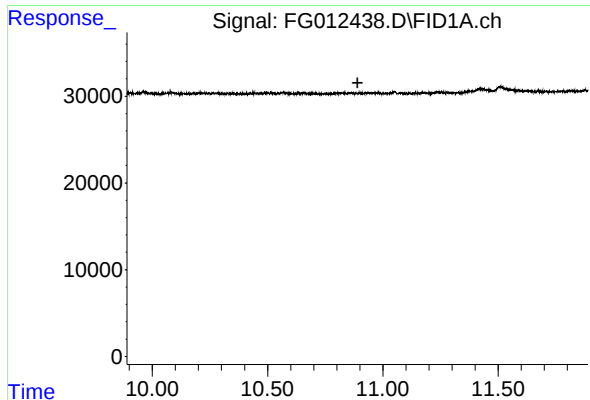

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 10.890 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

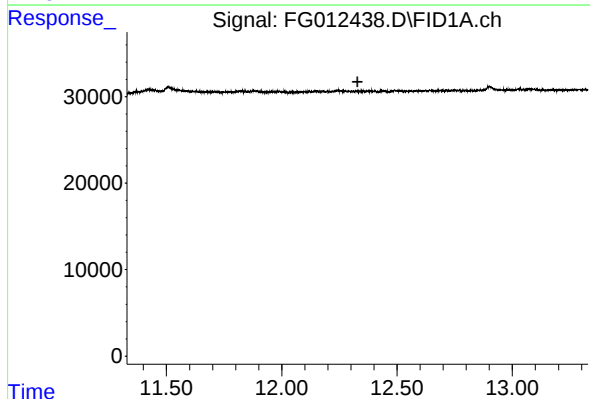


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.328 min
Response: 0
Conc: N.D.

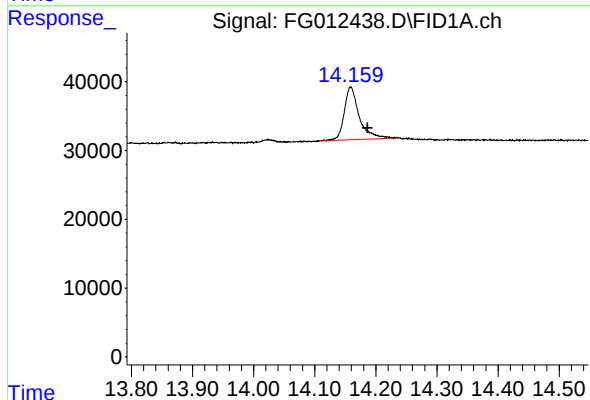


#14 n-Tetracosane (C24)

R.T.: 14.159 min
Delta R.T.: -0.028 min
Response: 131621
Conc: 0.94 ug/ml

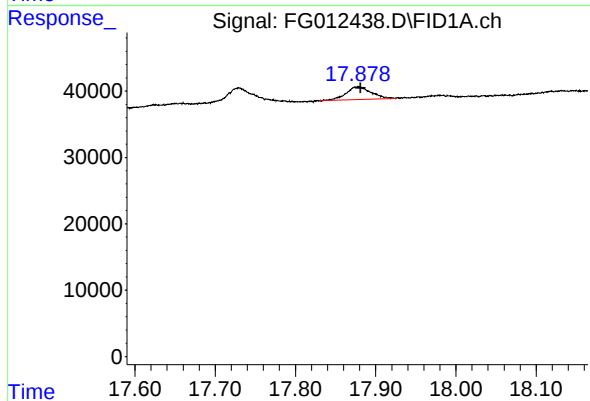

#18 n-Dotriacontane (C32)

R.T.: 17.878 min
Delta R.T.: -0.003 min
Response: 41935
Conc: 0.32 ug/ml

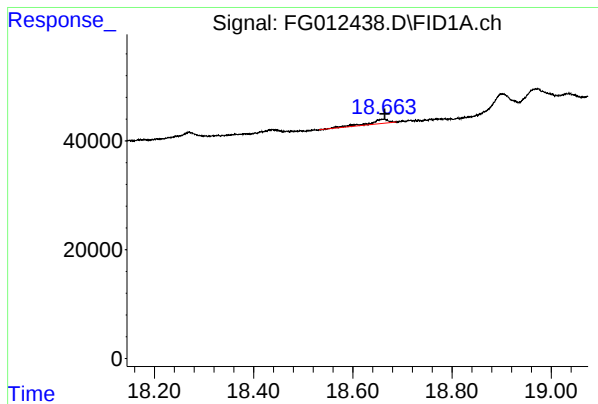

#19 n-Tetratriacontane (C34)

R.T.: 18.663 min
Delta R.T.: -0.002 min
Response: 22852
Conc: 0.18 ug/ml

Instrument :
FID_G
ClientSampleId :