

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071918\
 Data File : FG001733.D
 Signal(s) : FID1A.ch
 Acq On : 19 Jul 2018 16:38
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 20 02:05:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.515	5773476	49.624 ug/ml
Target Compounds			
2) N-DECANE	4.260	6674526	51.735 ug/ml
3) N-DODECANE	6.276	6730663	51.168 ug/ml
4) N-TETRADECANE	8.069	6736283	50.930 ug/ml
5) N-HEXADECANE	9.667	6767345	51.169 ug/ml
6) N-OCTADECANE	11.108	6809902	50.915 ug/ml
7) N-EICOSANE	12.418	6741734	50.505 ug/ml
8) N-DOCOSANE	13.616	6634967	49.862 ug/ml
10) N-TETRACOSANE	14.720	6473436	48.966 ug/ml
11) N-HEXACOSANE	15.741	6333032	48.103 ug/ml
12) N-OCTACOSANE	16.691	6237631	47.713 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071918\
Data File : FG001733.D
Signal(s) : FID1A.ch
Acq On : 19 Jul 2018 16:38
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 02:05:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

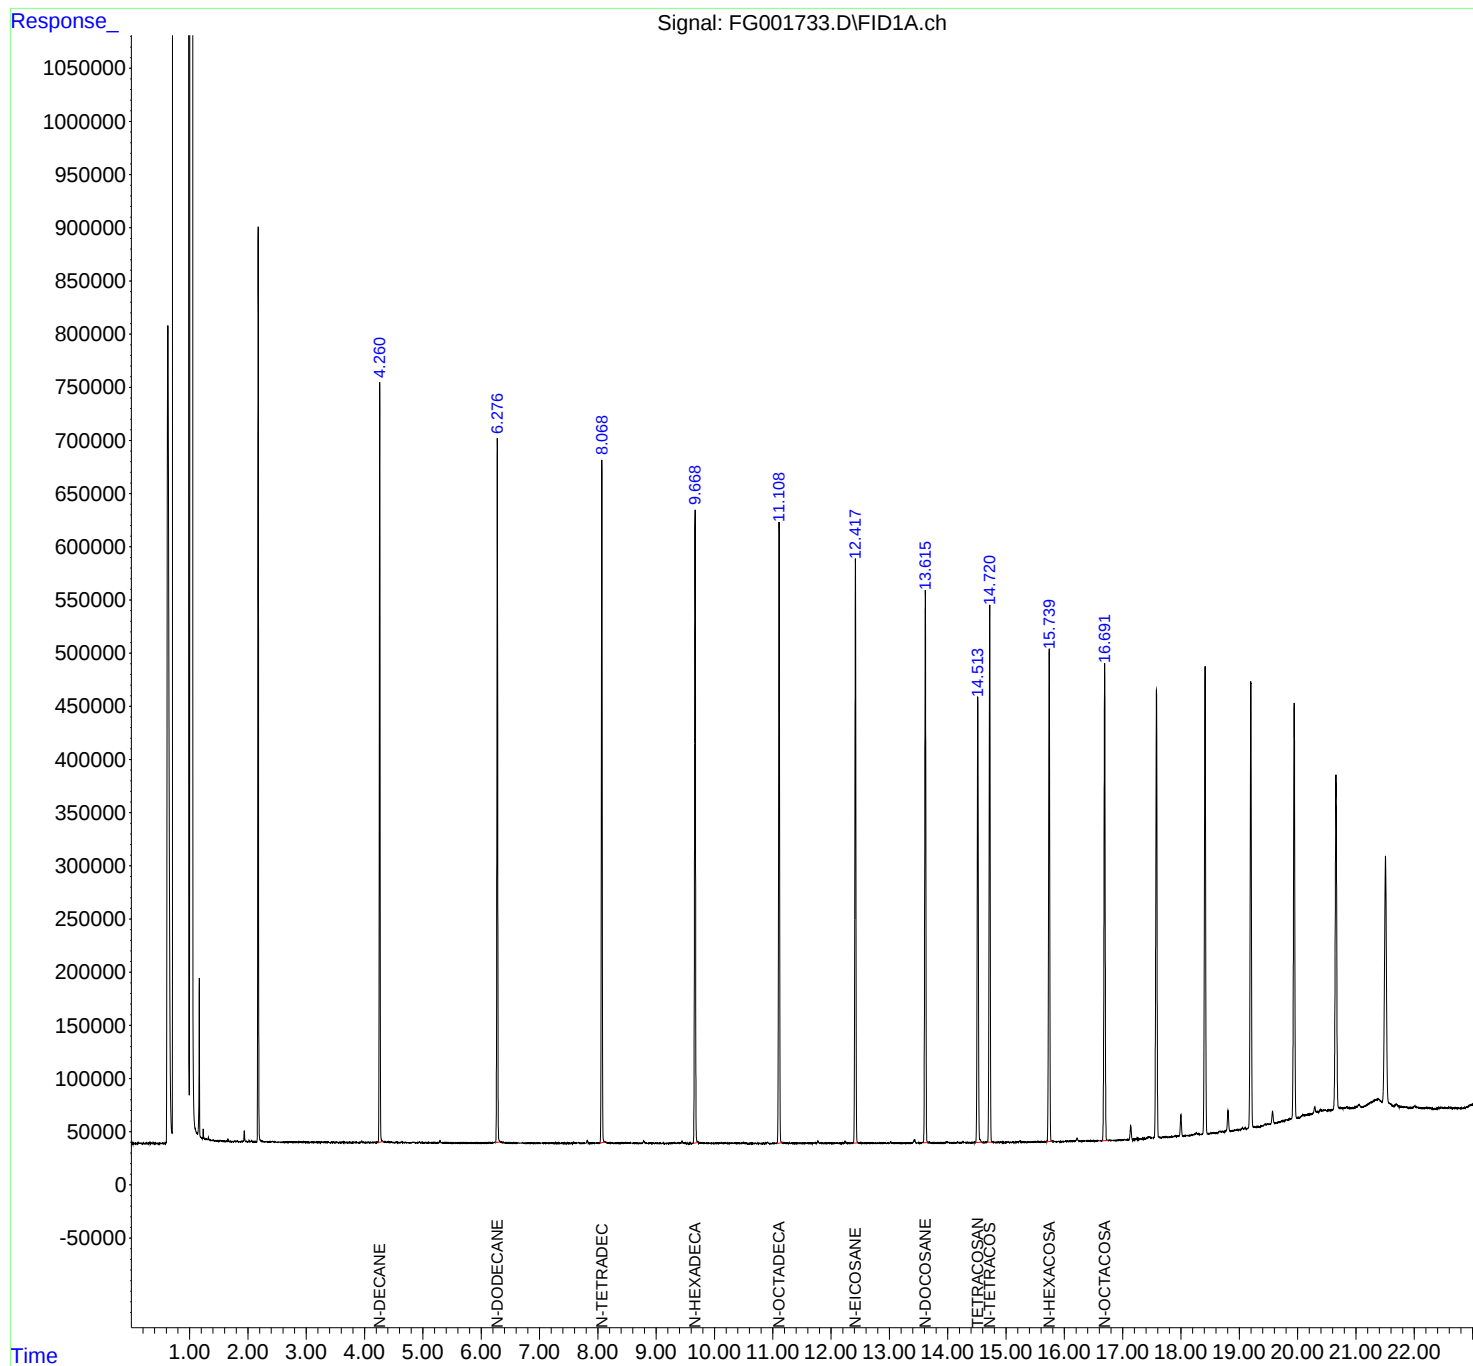

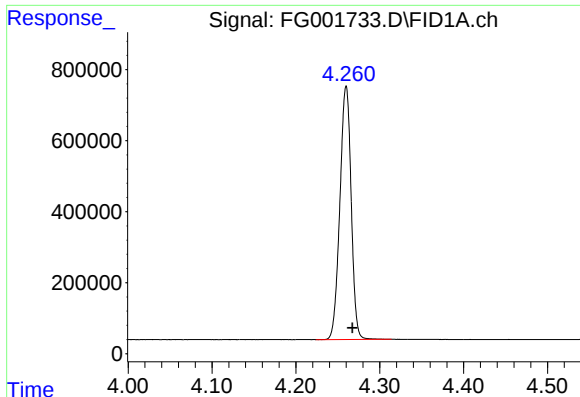


#2 N-DECANE

R.T.: 4.260 min
Delta R.T.: -0.007 min
Response: 6674526
Conc: 51.73 ug/ml

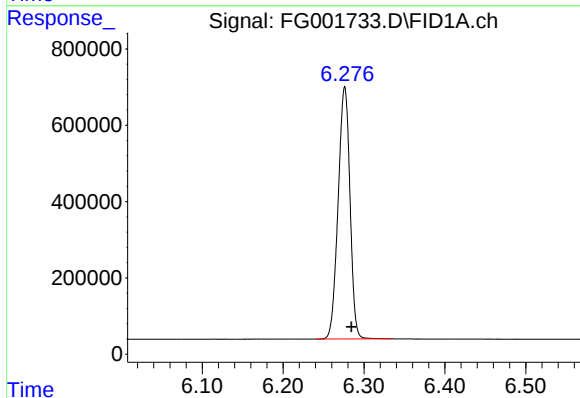


#3 N-DODECANE

R.T.: 6.276 min
Delta R.T.: -0.008 min
Response: 6730663
Conc: 51.17 ug/ml

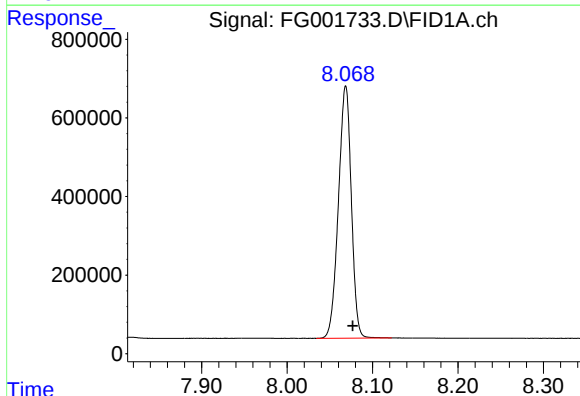


#4 N-TETRADECANE

R.T.: 8.069 min
Delta R.T.: -0.008 min
Response: 6736283
Conc: 50.93 ug/ml

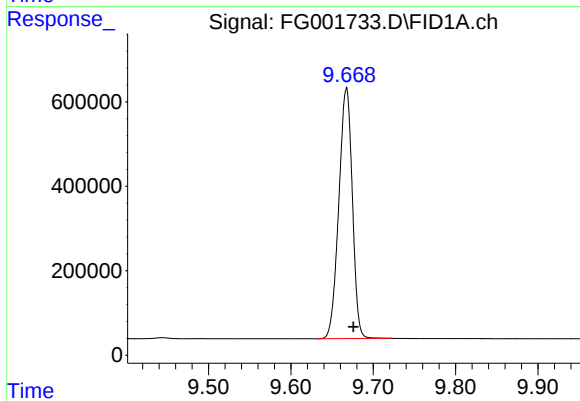


#5 N-HEXADECANE

R.T.: 9.667 min
Delta R.T.: -0.008 min
Response: 6767345
Conc: 51.17 ug/ml

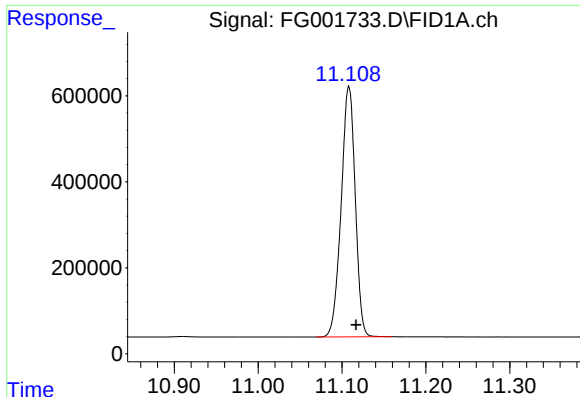


#6 N-OCTADECANE

R.T.: 11.108 min
Delta R.T.: -0.009 min
Response: 6809902
Conc: 50.91 ug/ml

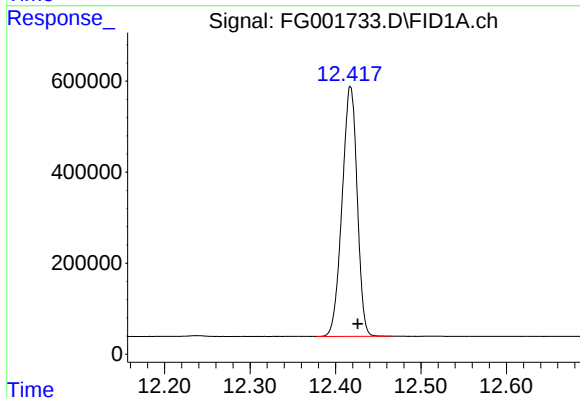


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: -0.009 min
Response: 6741734
Conc: 50.51 ug/ml

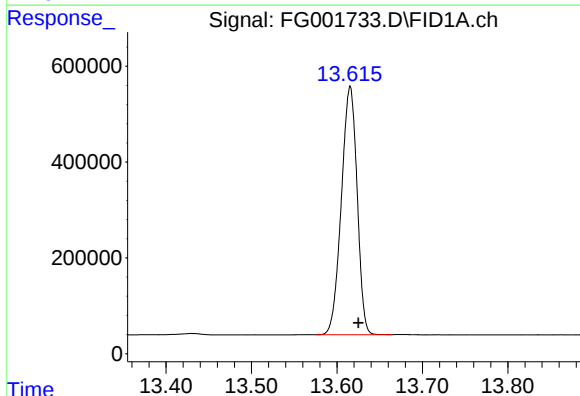


#8 N-DOCOSANE

R.T.: 13.616 min
Delta R.T.: -0.009 min
Response: 6634967
Conc: 49.86 ug/ml

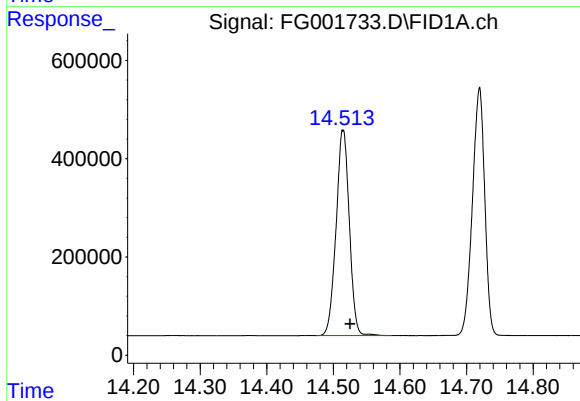


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.515 min
Delta R.T.: -0.011 min
Response: 5773476
Conc: 49.62 ug/ml

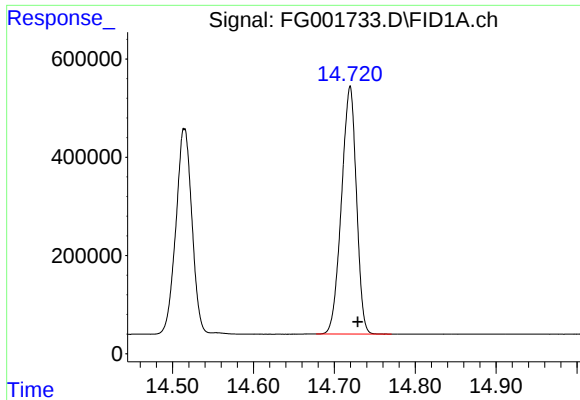


#10 N-TETRACOSANE

R.T.: 14.720 min
Delta R.T.: -0.009 min
Response: 6473436
Conc: 48.97 ug/ml

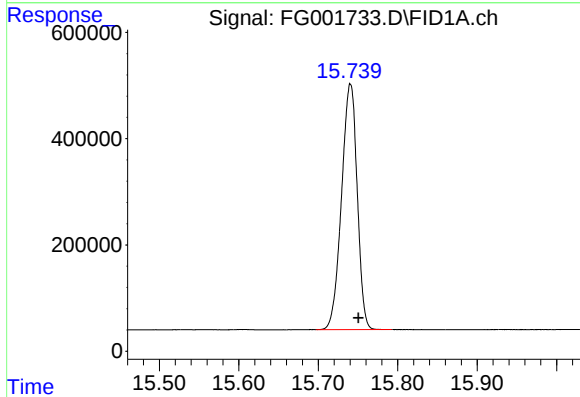

#11 N-HEXACOSANE

R.T.: 15.741 min
Delta R.T.: -0.010 min
Response: 6333032
Conc: 48.10 ug/ml

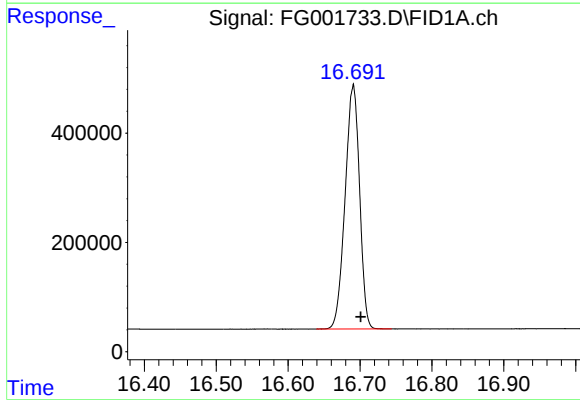

#12 N-OCTACOSANE

R.T.: 16.691 min
Delta R.T.: -0.010 min
Response: 6237631
Conc: 47.71 ug/ml