

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072023\
Data File : FG012500.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2023 13:13
Operator : YP\AJ
Sample : PB154312BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 04:18:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.975	1755161	16.424 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.156	218355	1.650 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072023\
Data File : FG012500.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2023 13:13
Operator : YP\AJ
Sample : PB154312BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 04:18:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

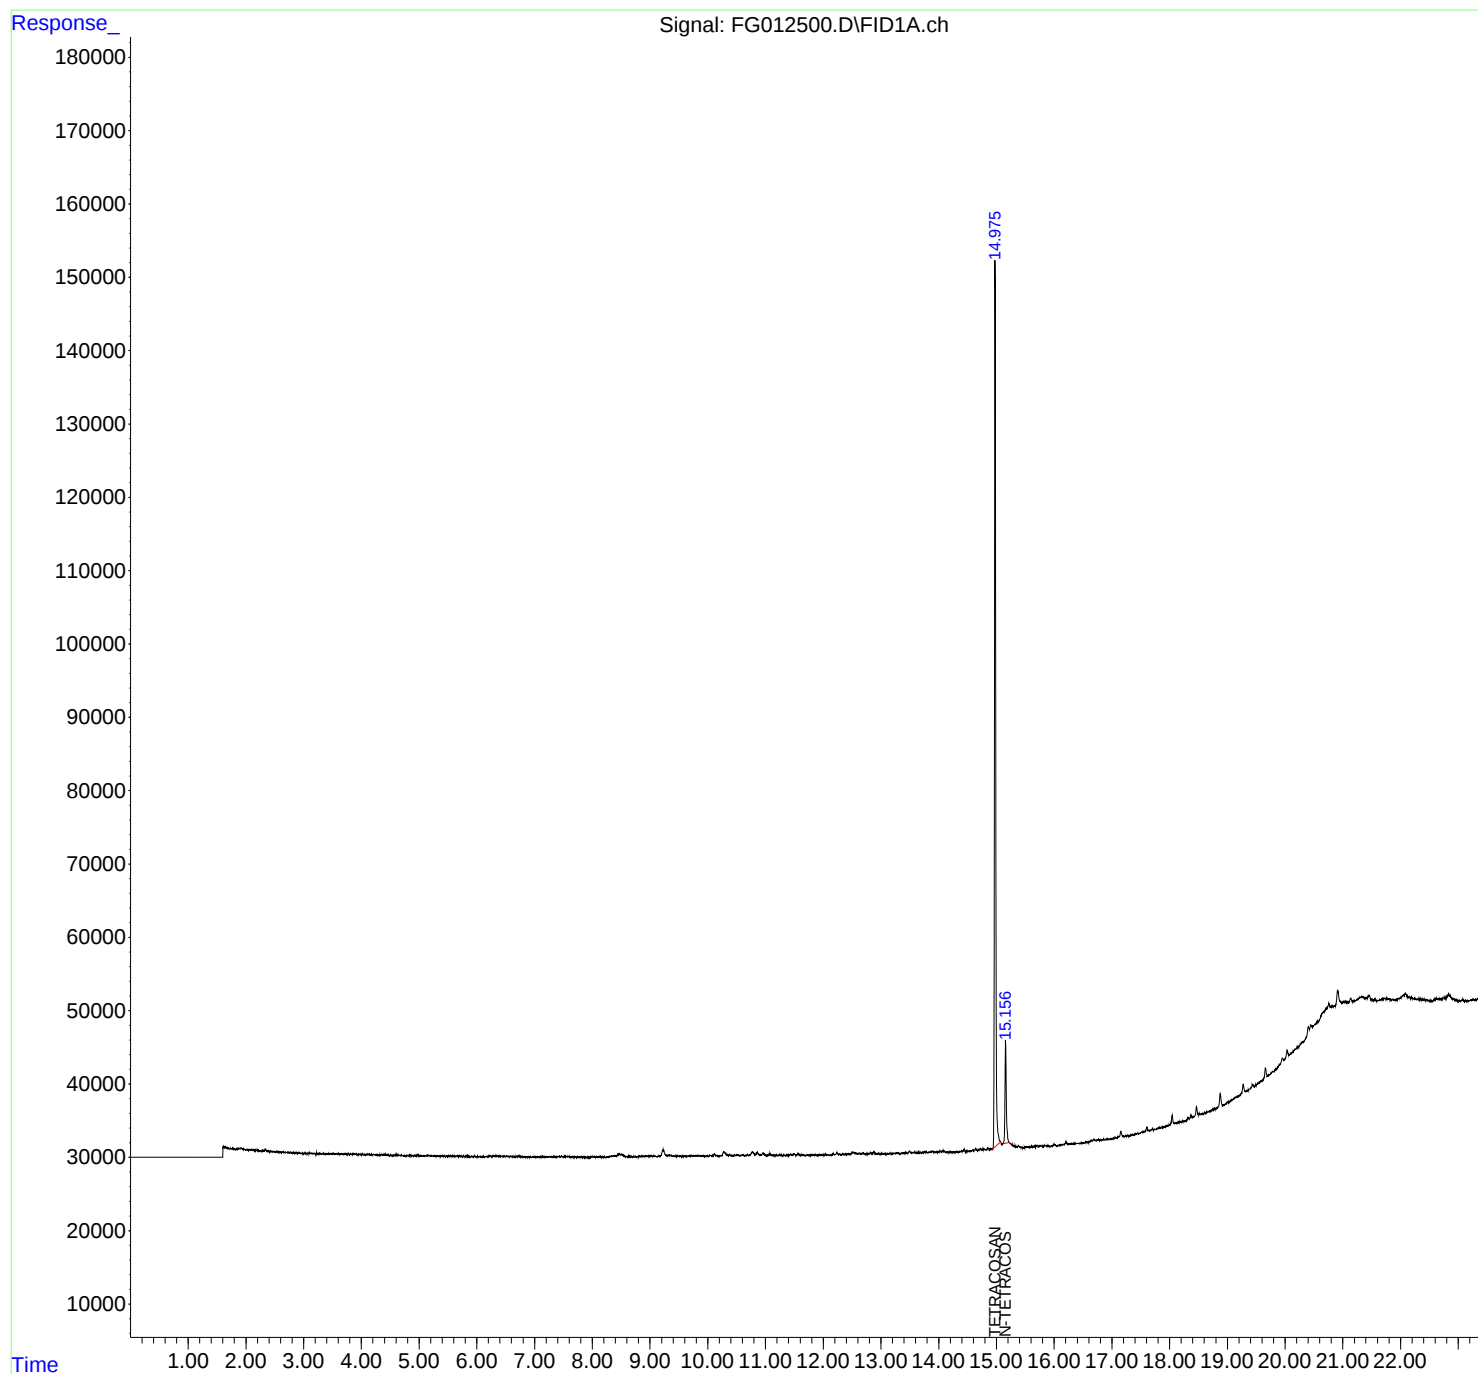


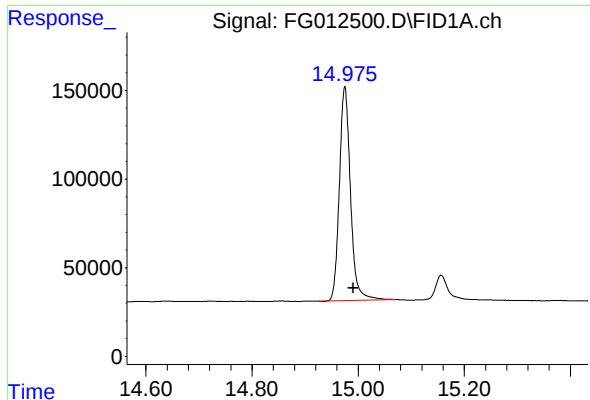

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.975 min
Delta R.T.: -0.016 min
Response: 1755161
Conc: 16.42 ug/ml

Instrument :
FID_G
ClientSampleId :

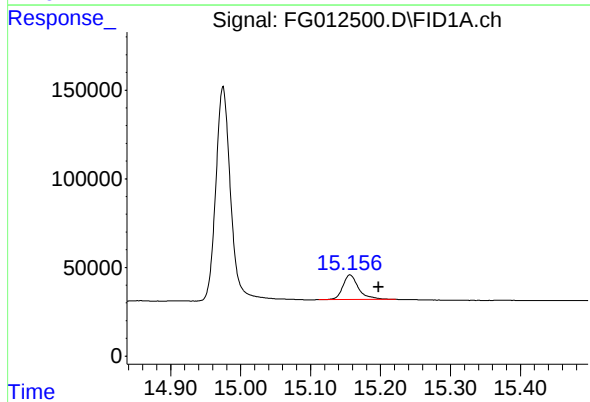

#10 N-TETRACOSANE

R.T.: 15.156 min
Delta R.T.: -0.041 min
Response: 218355
Conc: 1.65 ug/ml