

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072023AL\
 Data File : FG012488.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jul 2023 06:35
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 21 01:48:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 01:18:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	11.868	56874	0.421 ug/ml
11) T n-Heneicosane (C21)	12.485	49430	0.373 ug/ml
13) T n-Docosane (C22)	13.071	56250	0.427 ug/ml
14) T n-Tetracosane (C24)	14.156	2253599	16.046 ug/ml
15) T n-Hexacosane (C26)	15.199	48515	0.384 ug/ml
16) T n-Octacosane (C28)	16.151	55089	0.438 ug/ml
17) T n-Tricontane (C30)	17.039	62888	0.476 ug/ml
18) T n-Dotriacontane (C32)	17.872	157202	1.181 ug/ml
19) T n-Tetratriacontane (C34)	18.657	71370	0.557 ug/ml
20) T n-Hexatriacontane (C36)	19.401	41119	0.333 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072023AL\
Data File : FG012488.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2023 06:35
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 01:48:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

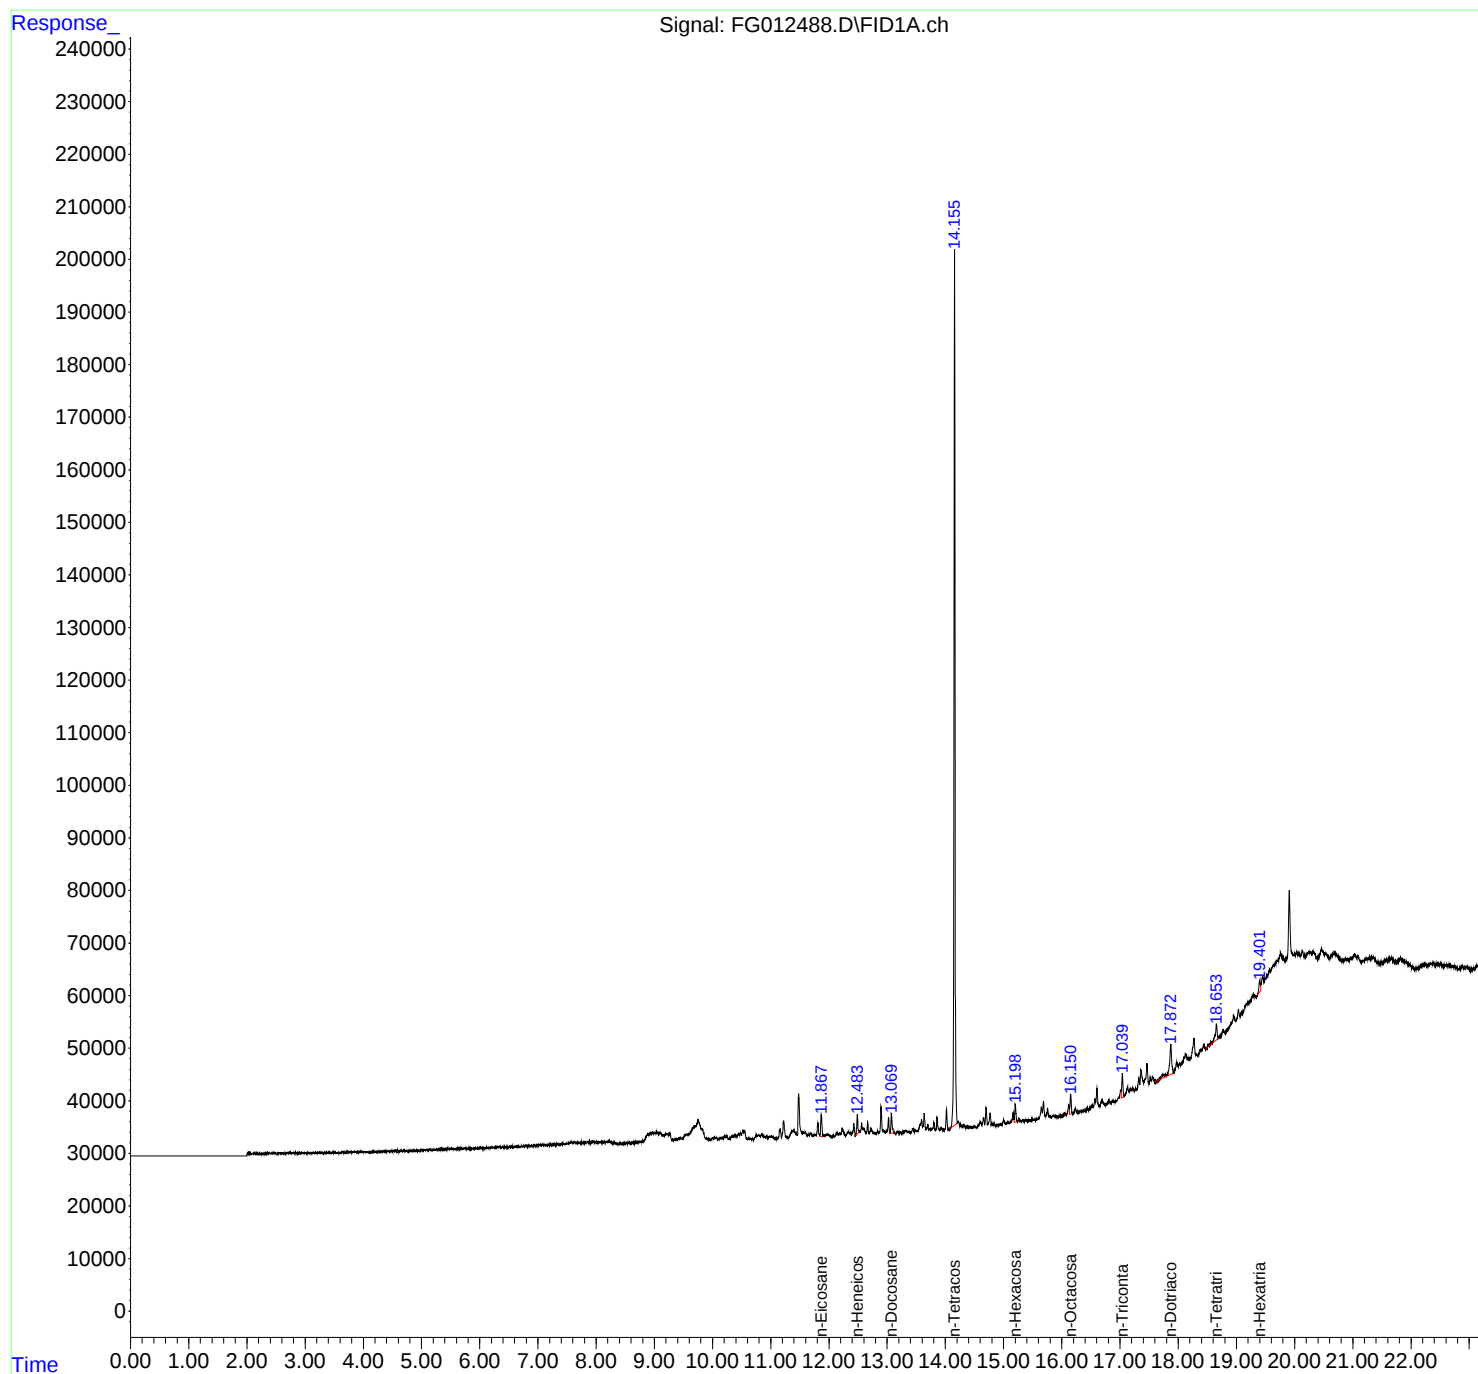


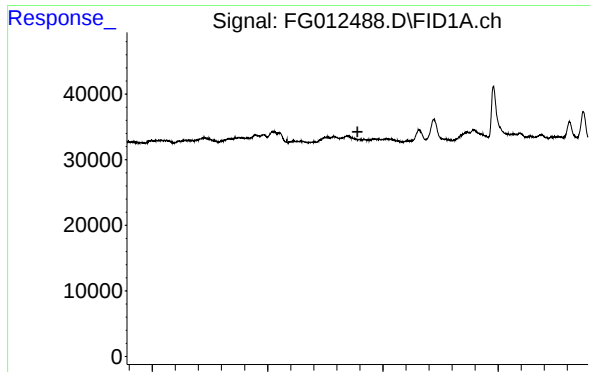

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.890 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

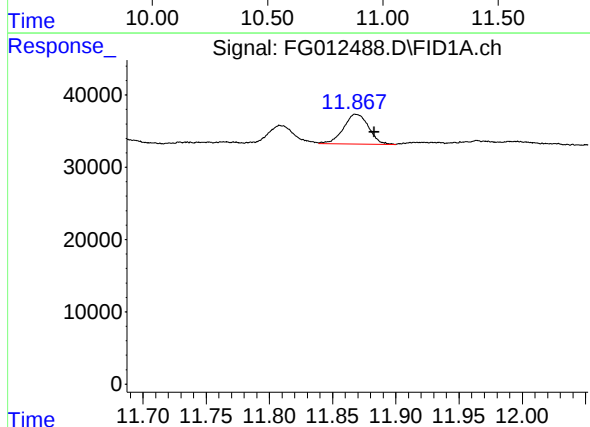


#10 n-Eicosane (C20)

R.T.: 11.868 min
Delta R.T.: -0.015 min
Response: 56874
Conc: 0.42 ug/ml

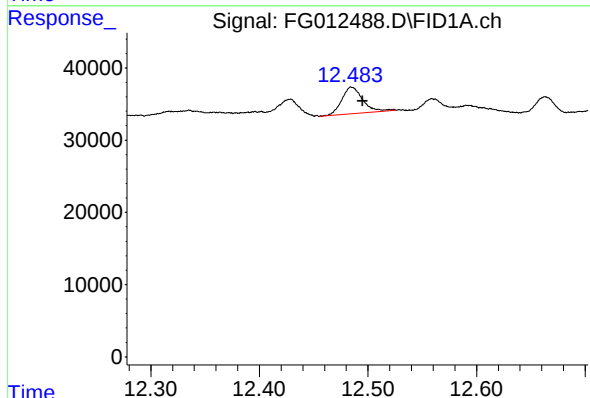


#11 n-Heneicosane (C21)

R.T.: 12.485 min
Delta R.T.: -0.010 min
Response: 49430
Conc: 0.37 ug/ml

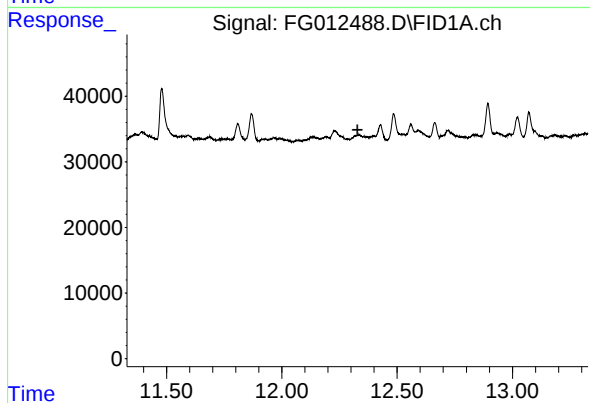

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.328 min
Response: 0
Conc: N.D.

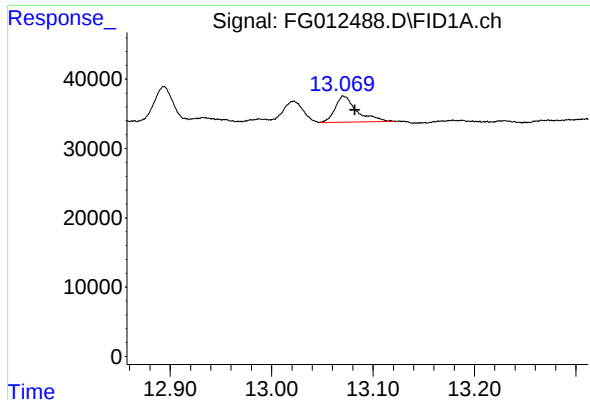

#13 n-Docosane (C22)


R.T.: 13.071 min
Delta R.T.: -0.011 min
Response: 56250
Conc: 0.43 ug/ml

Instrument :
FID_G
ClientSampleId :

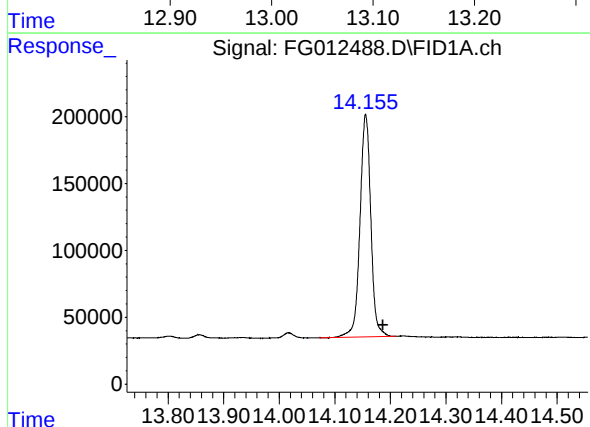


#14 n-Tetracosane (C24)

R.T.: 14.156 min
Delta R.T.: -0.031 min
Response: 2253599
Conc: 16.05 ug/ml

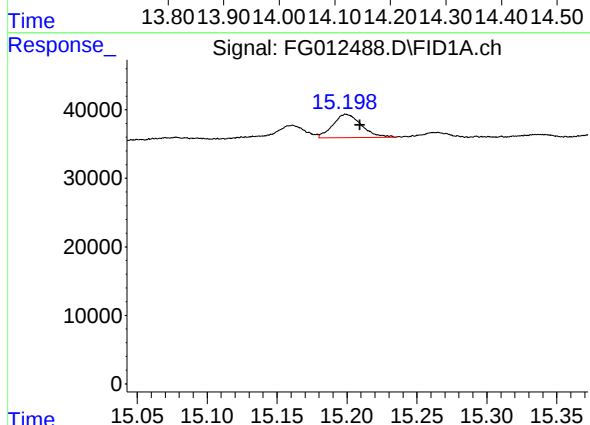


#15 n-Hexacosane (C26)

R.T.: 15.199 min
Delta R.T.: -0.010 min
Response: 48515
Conc: 0.38 ug/ml

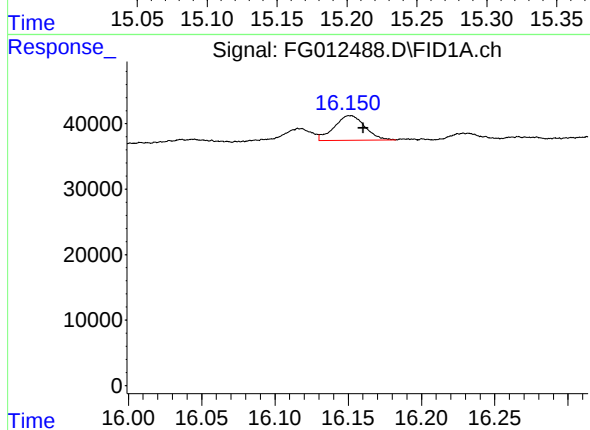

#16 n-Octacosane (C28)


R.T.: 16.151 min
Delta R.T.: -0.009 min
Response: 55089
Conc: 0.44 ug/ml

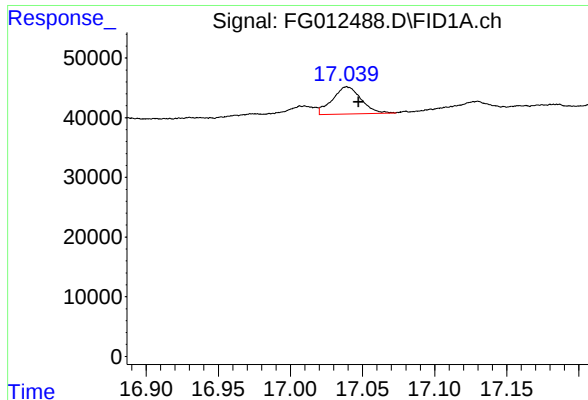

#17 n-Tricontane (C30)


R.T.: 17.039 min
Delta R.T.: -0.008 min
Response: 62888
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :

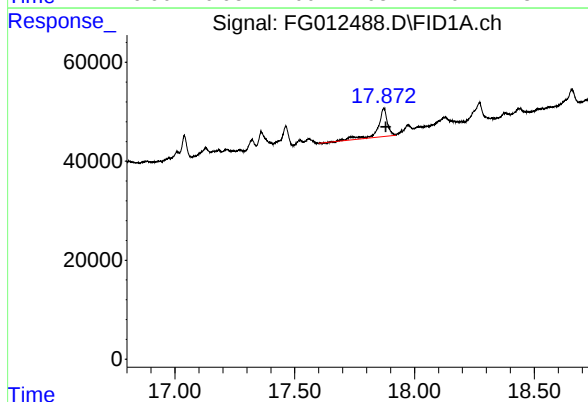


#18 n-Dotriacontane (C32)

R.T.: 17.872 min
Delta R.T.: -0.009 min
Response: 157202
Conc: 1.18 ug/ml

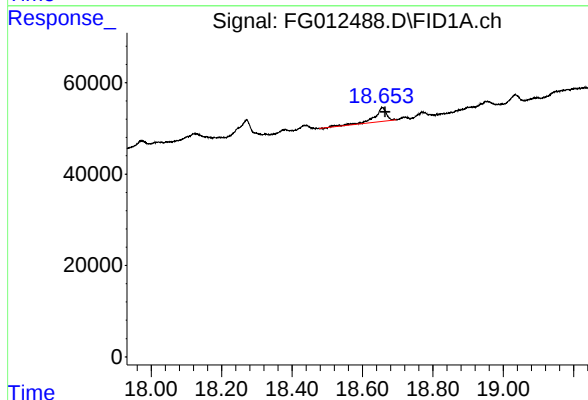

#19 n-Tetratriacontane (C34)

R.T.: 18.657 min
Delta R.T.: -0.009 min
Response: 71370
Conc: 0.56 ug/ml

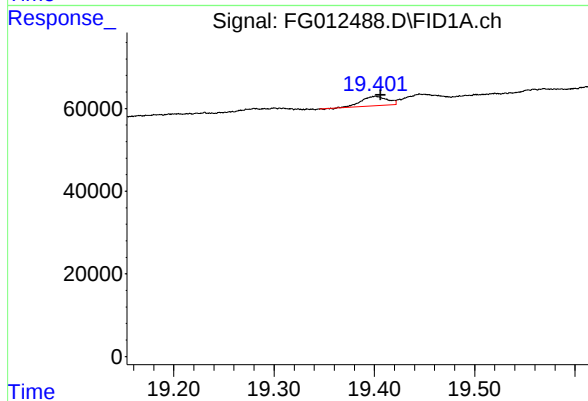

#20 n-Hexatriacontane (C36)

R.T.: 19.401 min
Delta R.T.: -0.005 min
Response: 41119
Conc: 0.33 ug/ml