

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG072123\  
Data File : FG012535.D  
Signal(s) : FID1A.ch  
Acq On : 21 Jul 2023 10:59  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 22 02:19:50 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG070623.M  
Quant Title :  
QLast Update : Thu Jul 06 13:57:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 7) N-EICOSANE               | 12.874 | 124984   | 0.989 ug/ml |
| 8) N-DOCOSANE               | 14.072 | 37783    | 0.308 ug/ml |
| 10) N-TETRACOSANE           | 15.157 | 1223403  | 9.247 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG072123\  
Data File : FG012535.D  
Signal(s) : FID1A.ch  
Acq On : 21 Jul 2023 10:59  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 22 02:19:50 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG070623.M  
Quant Title :  
QLast Update : Thu Jul 06 13:57:02 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

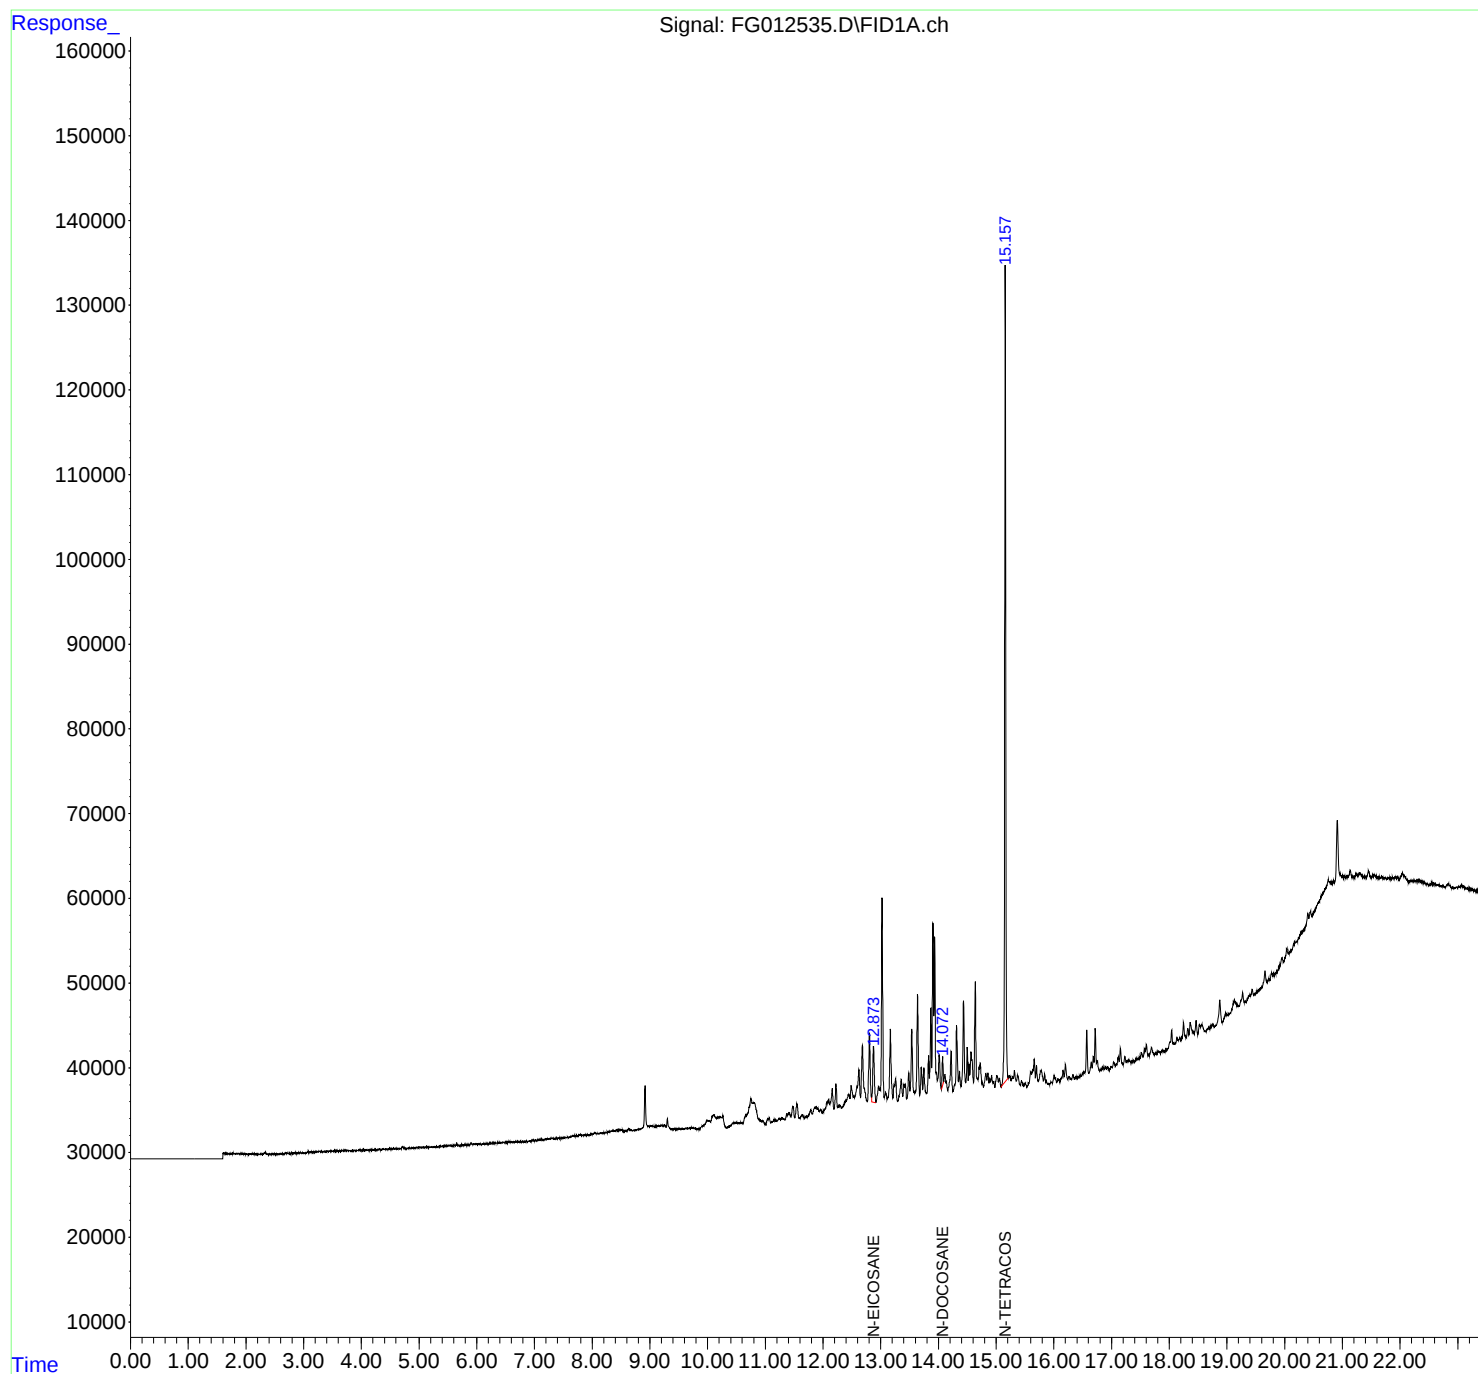


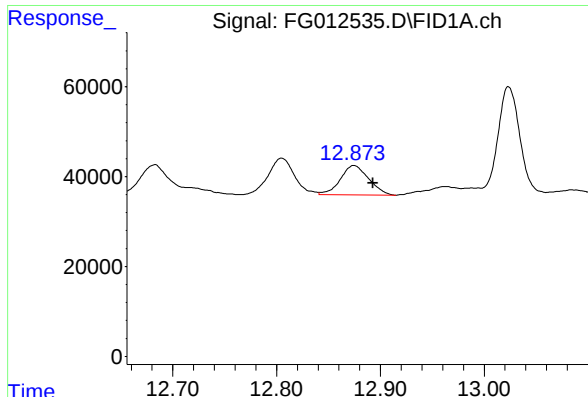

#7 N-EICOSANE


R.T.: 12.874 min  
Delta R.T.: -0.018 min  
Response: 124984  
Conc: 0.99 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

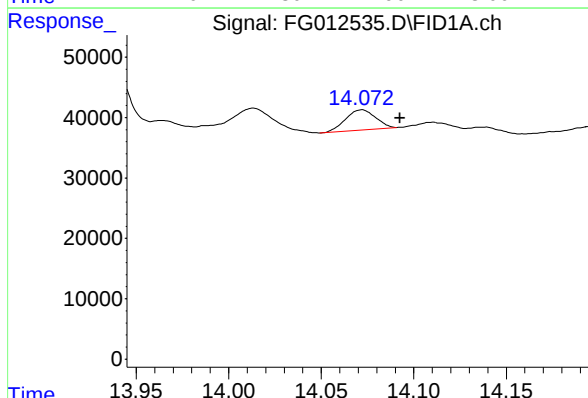


#8 N-DOCOSANE

R.T.: 14.072 min  
Delta R.T.: -0.021 min  
Response: 37783  
Conc: 0.31 ug/ml

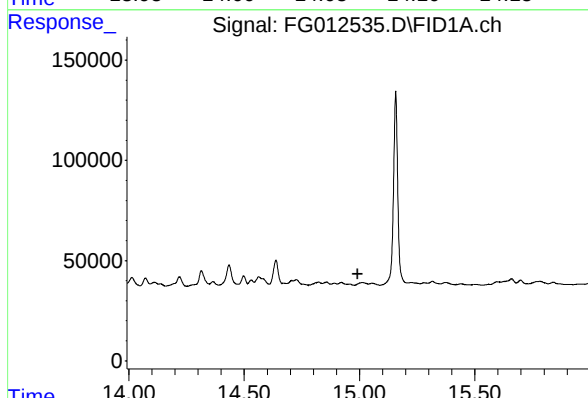

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.991 min  
Response: 0  
Conc: N.D.

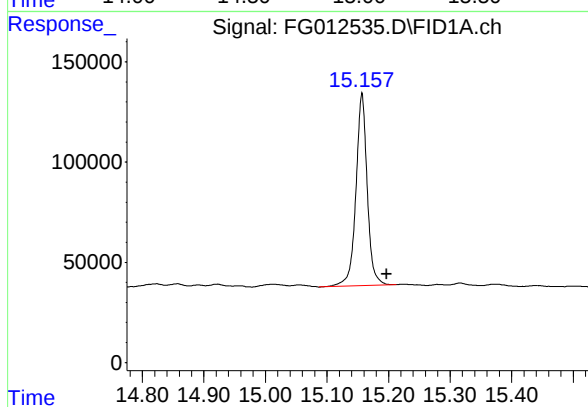

#10 N-TETRACOSANE

R.T.: 15.157 min  
Delta R.T.: -0.040 min  
Response: 1223403  
Conc: 9.25 ug/ml