

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072123\
Data File : FG012545.D
Signal(s) : FID1A.ch
Acq On : 21 Jul 2023 19:28
Operator : YP\AJ
Sample : 03681-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RPTP-6-CS-6

Integration File: autoint1.e
Quant Time: Jul 22 02:20:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.975	1160508	10.860 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072123\
Data File : FG012545.D
Signal(s) : FID1A.ch
Acq On : 21 Jul 2023 19:28
Operator : YP\AJ
Sample : 03681-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RPTP-6-CS-6

Integration File: autoint1.e
Quant Time: Jul 22 02:20:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

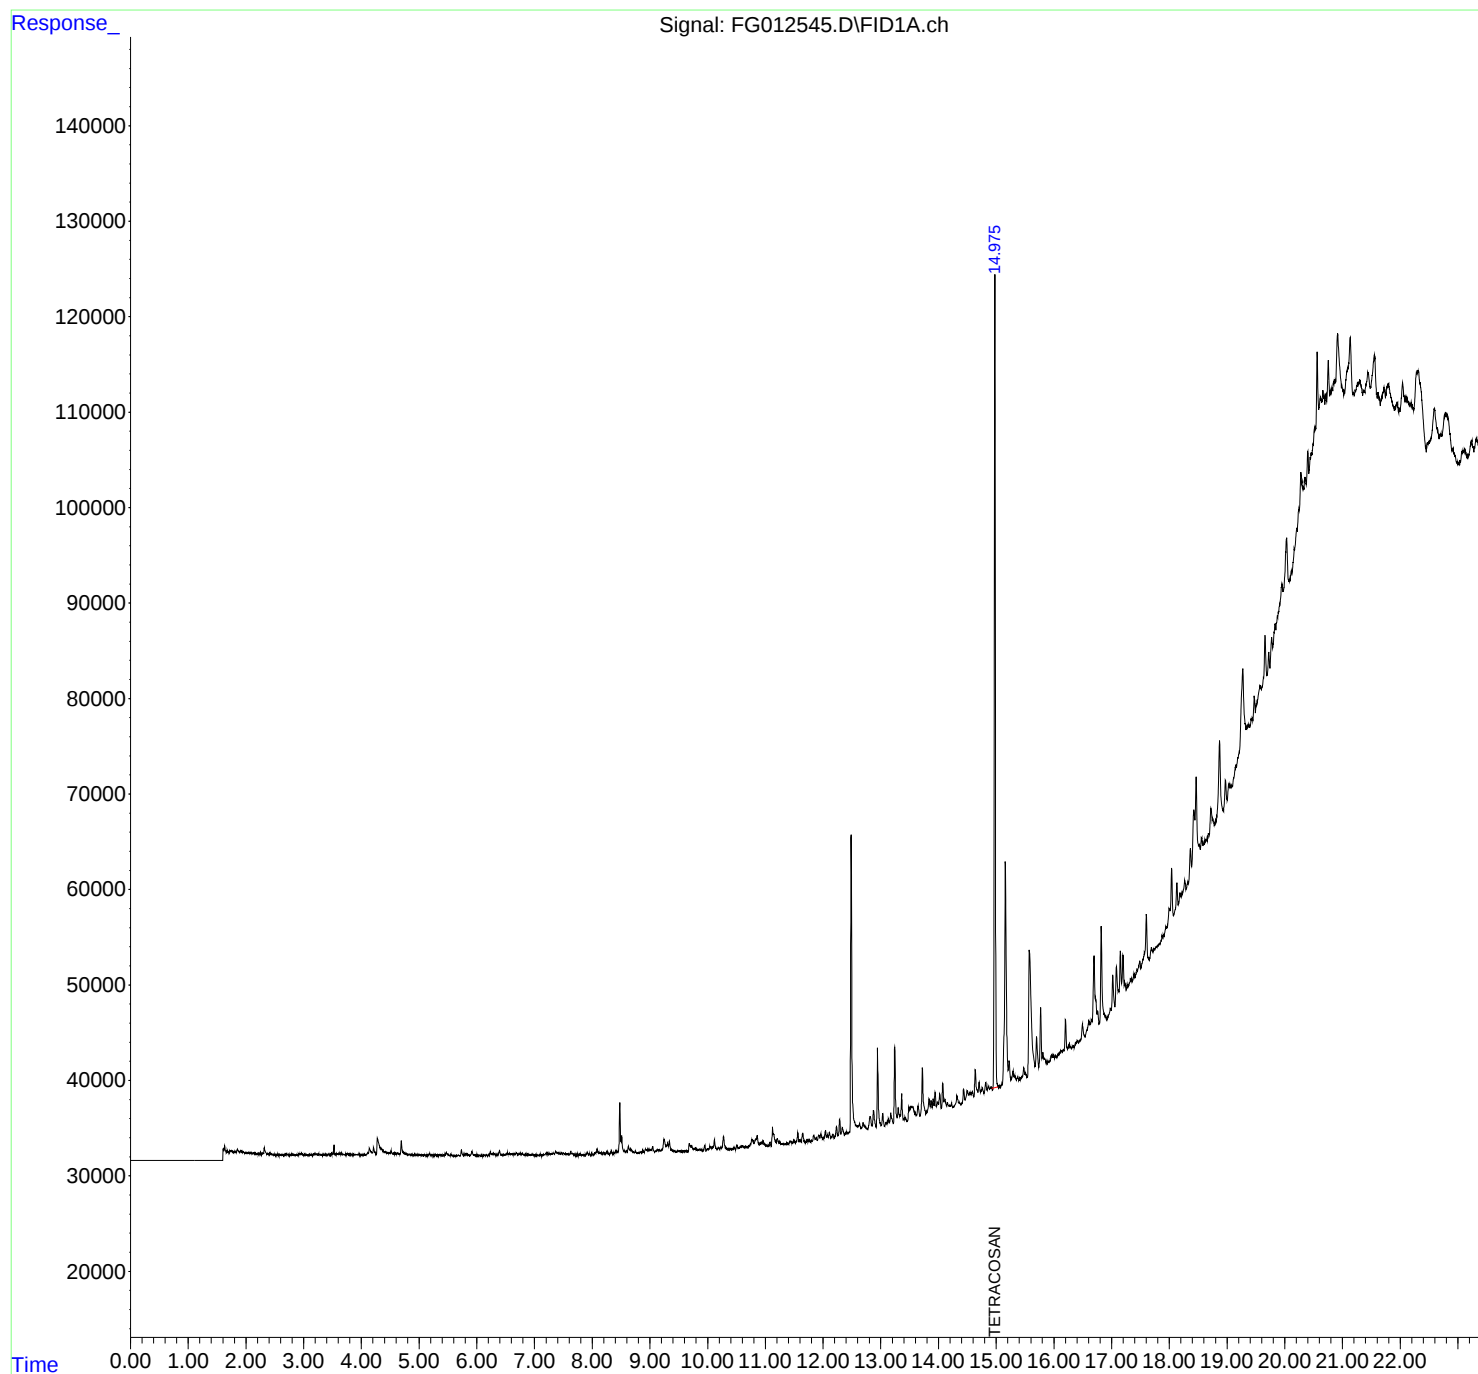

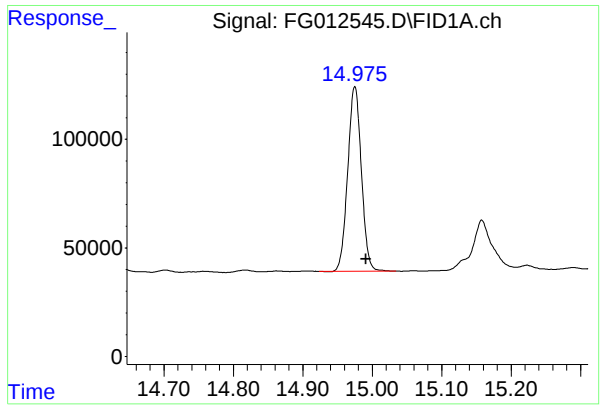

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.975 min
Delta R.T.: -0.016 min
Response: 1160508
Conc: 10.86 ug/ml

Instrument :
FID_G
ClientSampleId :
RPTP-6-CS-6