

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072123AL\
 Data File : FG012508.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jul 2023 18:39
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 21 05:46:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 01:18:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	13.041	128383	0.974 ug/ml
14) T	n-Tetracosane (C24)	14.229	46442	0.331 ug/ml
15) T	n-Hexacosane (C26)	15.166	276090	2.187 ug/ml
16) T	n-Octacosane (C28)	16.163	257630	2.049 ug/ml
20) T	n-Hexatriacontane (C36)	19.456	21295	0.172 ug/ml
22) T	n-Tetracontane (C40)	21.016	21469	0.185 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072123AL\
Data File : FG012508.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2023 18:39
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 05:46:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

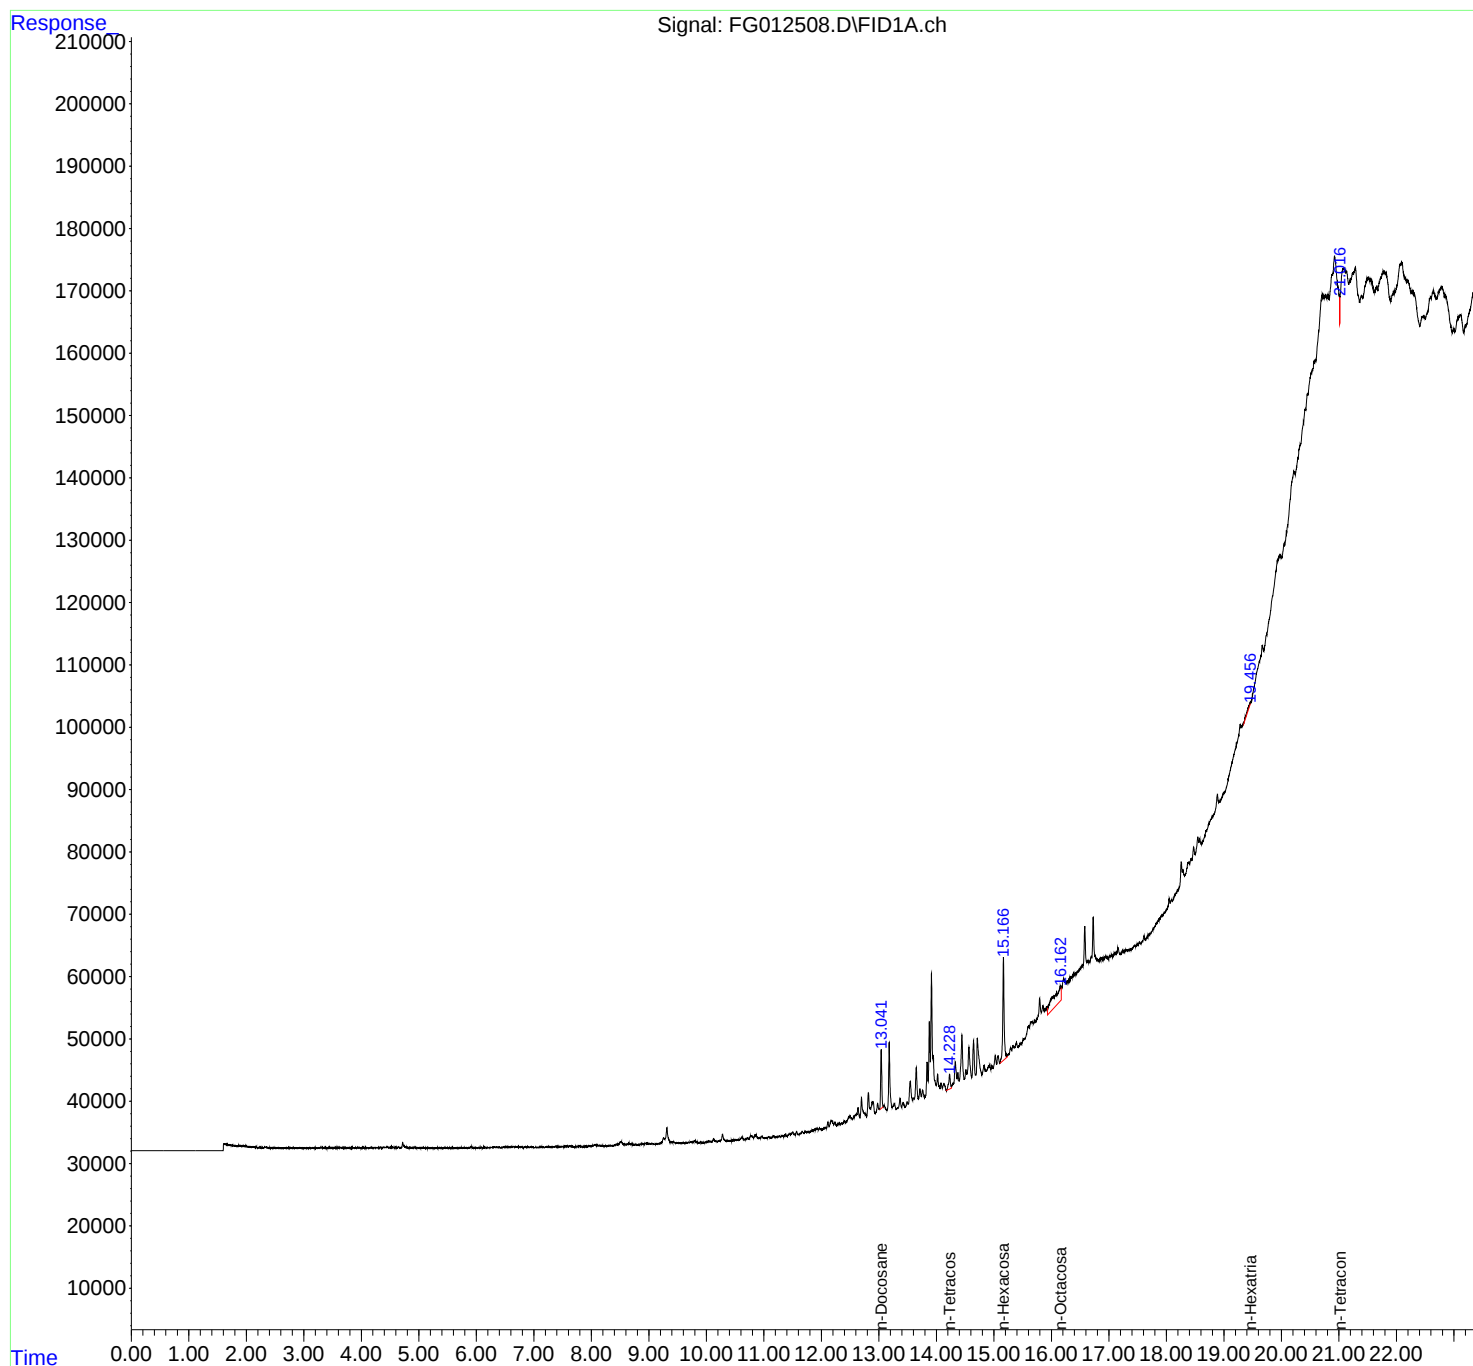


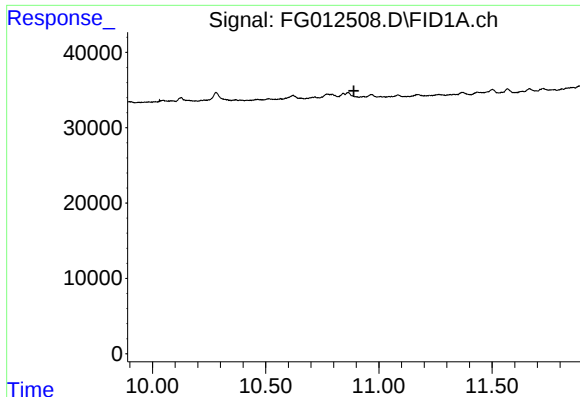

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.890 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

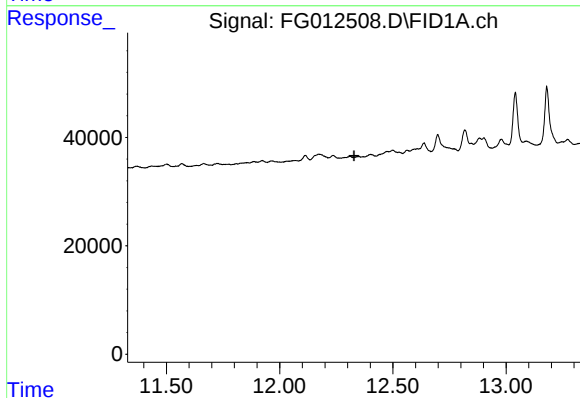


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.328 min
Response: 0
Conc: N.D.

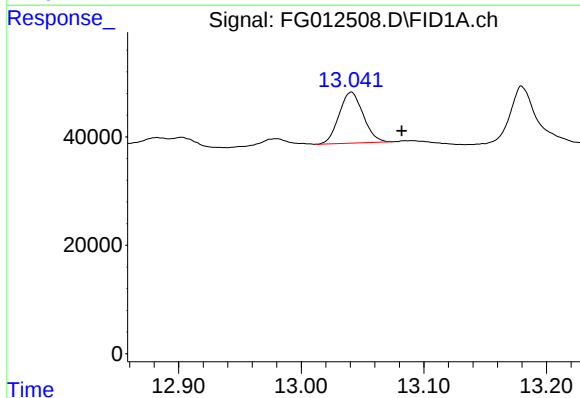


#13 n-Docosane (C22)

R.T.: 13.041 min
Delta R.T.: -0.041 min
Response: 128383
Conc: 0.97 ug/ml

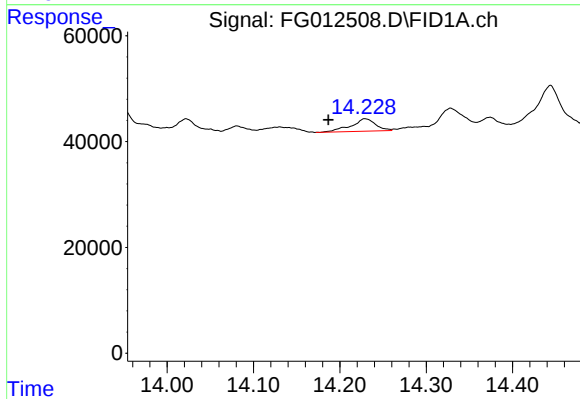

#14 n-Tetracosane (C24)


R.T.: 14.229 min
Delta R.T.: 0.042 min
Response: 46442
Conc: 0.33 ug/ml

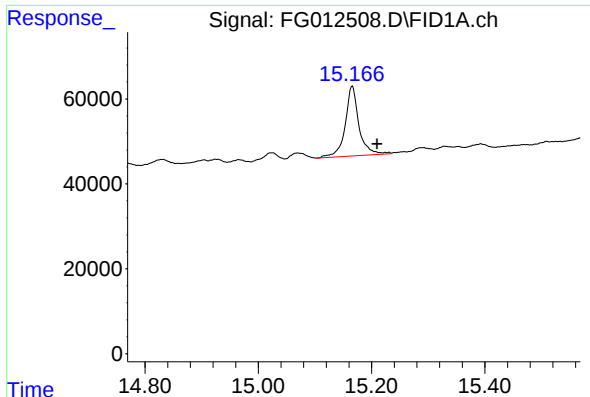

#15 n-Hexacosane (C26)


R.T.: 15.166 min
Delta R.T.: -0.044 min
Response: 276090
Conc: 2.19 ug/ml

Instrument :
FID_G
ClientSampleId :

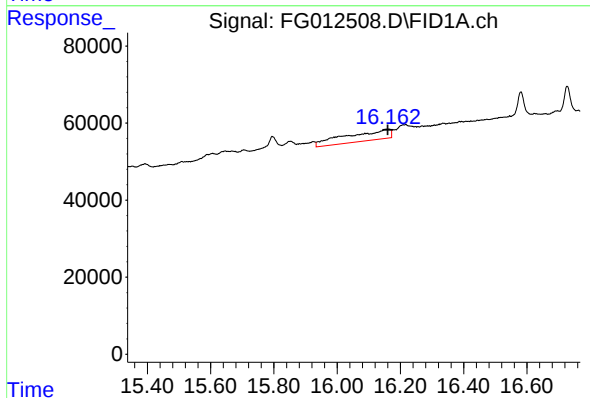


#16 n-Octacosane (C28)

R.T.: 16.163 min
Delta R.T.: 0.002 min
Response: 257630
Conc: 2.05 ug/ml

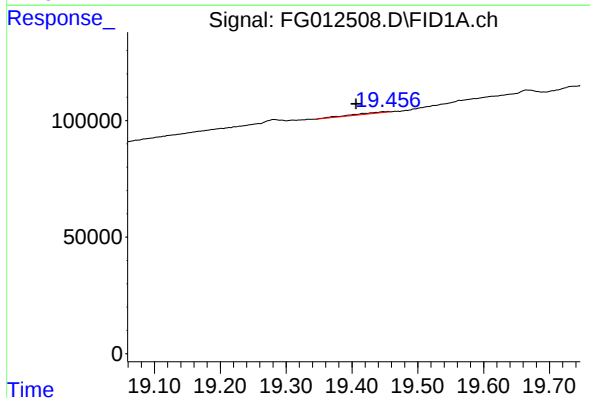

#20 n-Hexatriacontane (C36)

R.T.: 19.456 min
Delta R.T.: 0.050 min
Response: 21295
Conc: 0.17 ug/ml

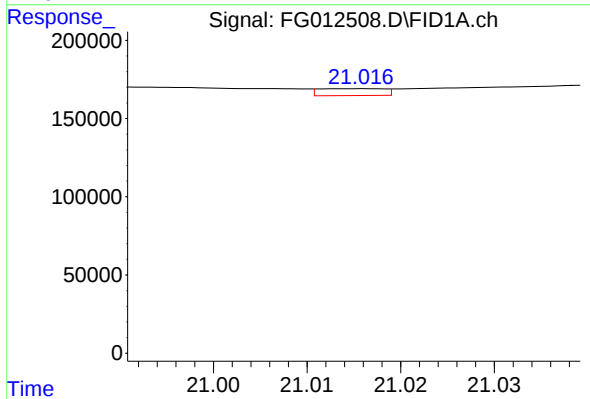

#22 n-Tetracontane (C40)

R.T.: 21.016 min
Delta R.T.: -0.032 min
Response: 21469
Conc: 0.19 ug/ml