

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072123AL\
 Data File : FG012509.D
 Signal(s) : FID1A.ch
 Acq On : 20 Jul 2023 19:08
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 21 05:46:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 15 01:18:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	11.818f	30055	0.222 ug/ml
11) T n-Heneicosane (C21)	12.545	44278	0.334 ug/ml
14) T n-Tetracosane (C24)	14.165	191041	1.360 ug/ml
15) T n-Hexacosane (C26)	15.207	35596	0.282 ug/ml
16) T n-Octacosane (C28)	16.159	30886	0.246 ug/ml
17) T n-Tricontane (C30)	17.047	2060	0.016 ug/ml
18) T n-Dotriacontane (C32)	17.883	73589	0.553 ug/ml
19) T n-Tetratriacontane (C34)	18.665	102664	0.801 ug/ml
20) T n-Hexatriacontane (C36)	19.447	107222	0.868 ug/ml
22) T n-Tetracontane (C40)	21.089	266787	2.302 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072123AL\
Data File : FG012509.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2023 19:08
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 21 05:46:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 071423.M
Quant Title : GC Extractables
QLast Update : Sat Jul 15 01:18:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

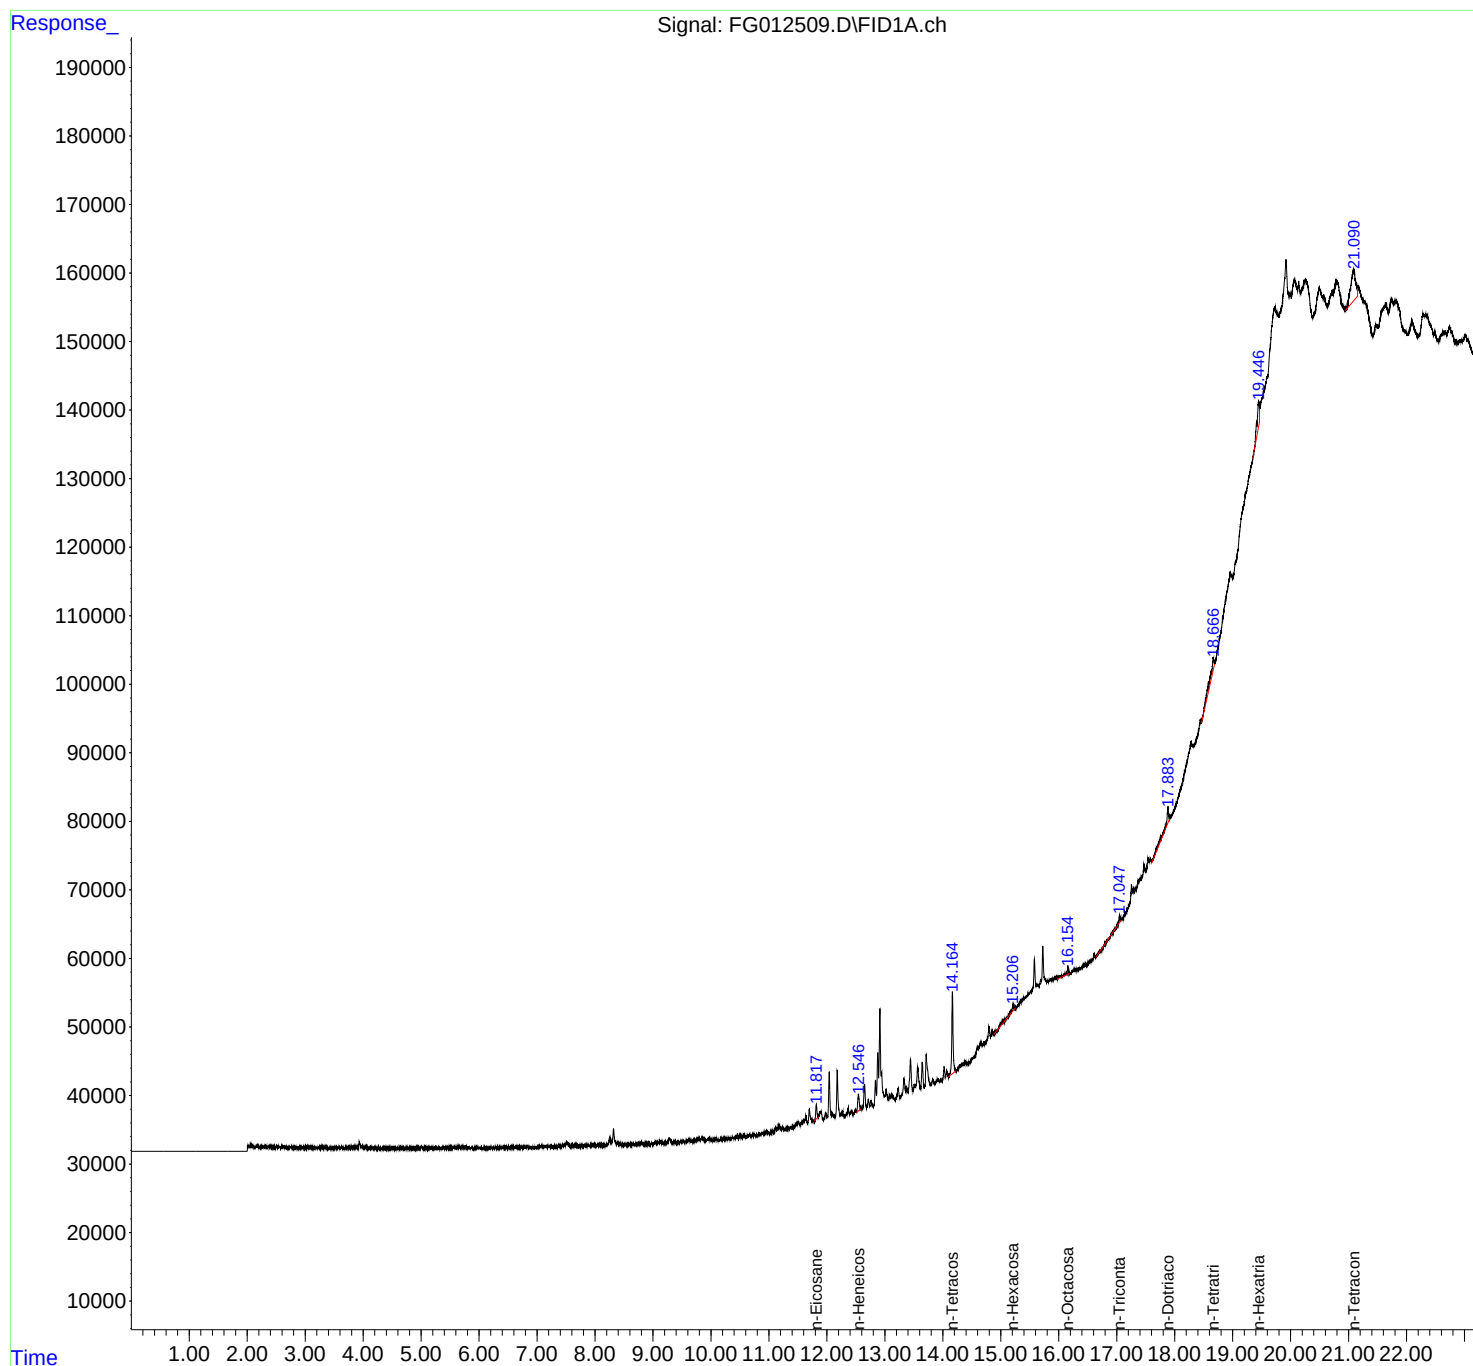


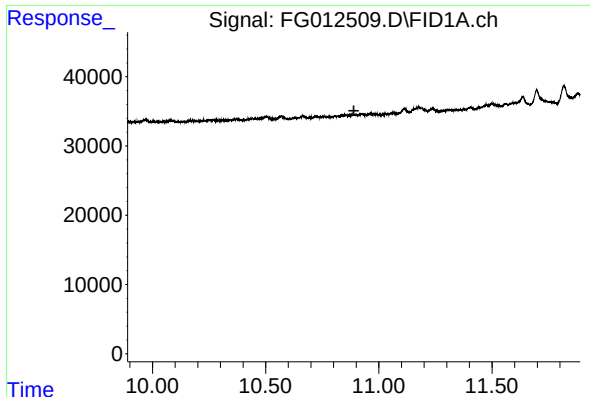

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.890 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

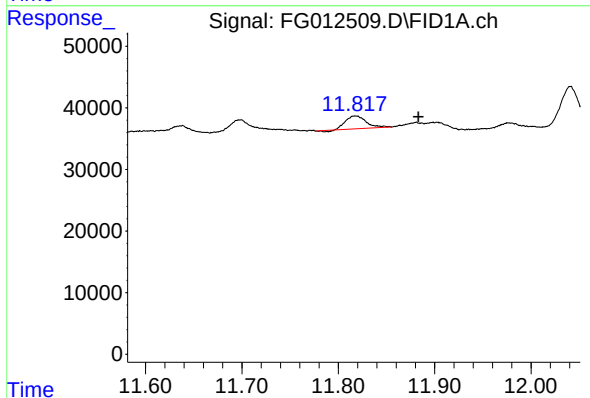


#10 n-Eicosane (C20)

R.T.: 11.818 min
Delta R.T.: -0.065 min
Response: 30055
Conc: 0.22 ug/ml

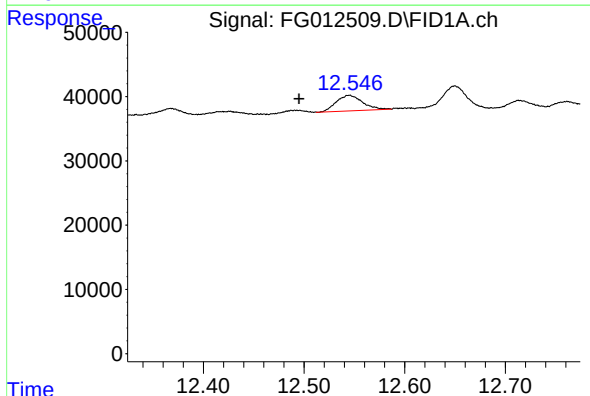


#11 n-Heneicosane (C21)

R.T.: 12.545 min
Delta R.T.: 0.050 min
Response: 44278
Conc: 0.33 ug/ml

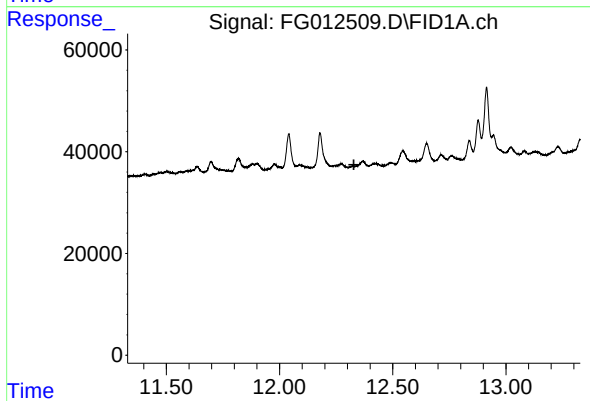

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.328 min
Response: 0
Conc: N.D.

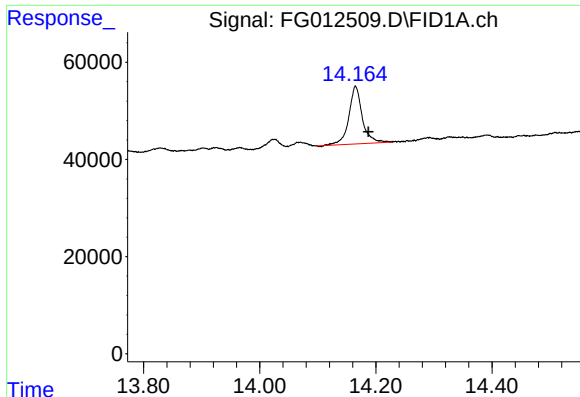

#14 n-Tetracosane (C24)


R.T.: 14.165 min
Delta R.T.: -0.022 min
Response: 191041
Conc: 1.36 ug/ml

Instrument :
FID_G
ClientSampleId :

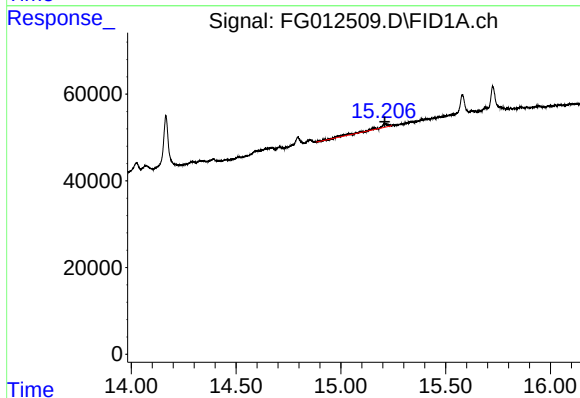


#15 n-Hexacosane (C26)

R.T.: 15.207 min
Delta R.T.: -0.003 min
Response: 35596
Conc: 0.28 ug/ml

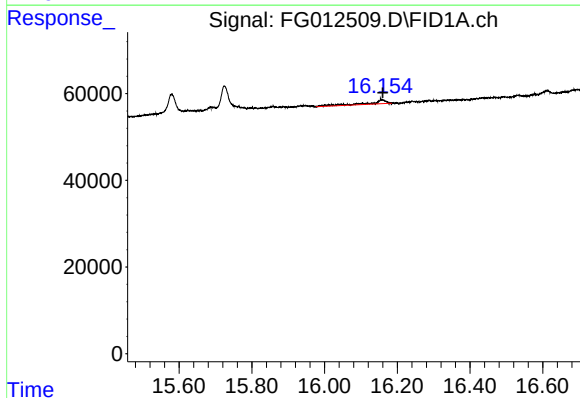


#16 n-Octacosane (C28)

R.T.: 16.159 min
Delta R.T.: -0.001 min
Response: 30886
Conc: 0.25 ug/ml

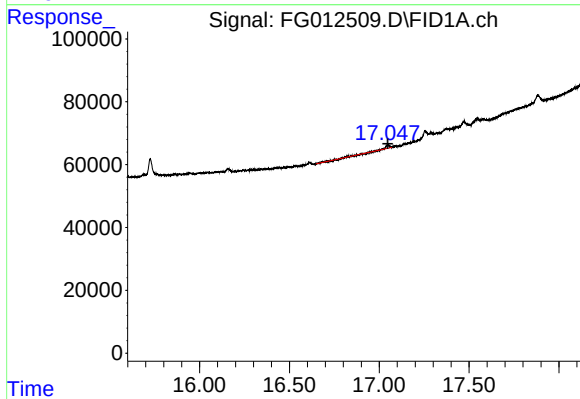

#17 n-Tricontane (C30)


R.T.: 17.047 min
Delta R.T.: 0.000 min
Response: 2060
Conc: 0.02 ug/ml

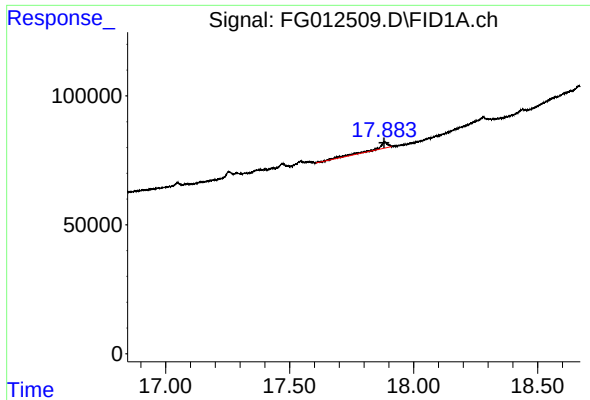

#18 n-Dotriacontane (C32)


R.T.: 17.883 min
Delta R.T.: 0.002 min
Response: 73589
Conc: 0.55 ug/ml

Instrument :
FID_G
ClientSampleId :

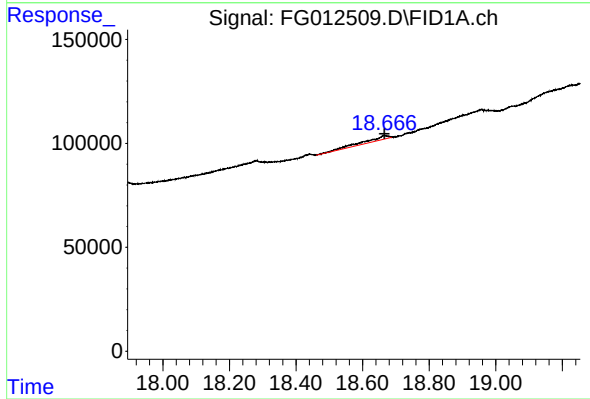


#19 n-Tetratriacontane (C34)

R.T.: 18.665 min
Delta R.T.: 0.000 min
Response: 102664
Conc: 0.80 ug/ml

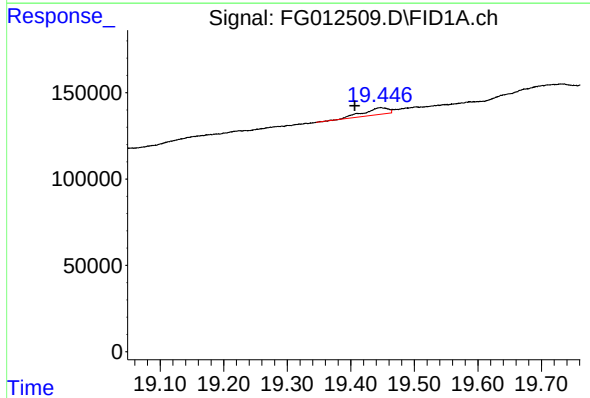

#20 n-Hexatriacontane (C36)

R.T.: 19.447 min
Delta R.T.: 0.041 min
Response: 107222
Conc: 0.87 ug/ml

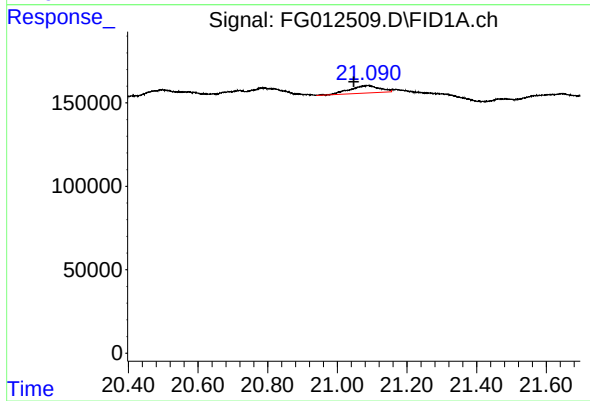

#22 n-Tetracontane (C40)

R.T.: 21.089 min
Delta R.T.: 0.041 min
Response: 266787
Conc: 2.30 ug/ml