

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072318\
 Data File : FG001750.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jul 2018 14:32
 Operator : AJ\SJ
 Sample : J4081-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 24 05:05:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.507	2312094	19.873 ug/ml
Target Compounds			
4) N-TETRADECANE	8.120	538373	4.070 ug/ml
7) N-EICOSANE	12.408	107899	0.808 ug/ml
8) N-DOCOSANE	13.619	172087	1.293 ug/ml
10) N-TETRACOSANE	14.674f	913994	6.914 ug/ml
11) N-HEXACOSANE	15.730	274709	2.087 ug/ml
12) N-OCTACOSANE	16.679	432727	3.310 ug/ml
13) N-TRIACONTANE	17.567	284344	2.182 ug/ml
14) N-DOTRIACONTANE	18.396	179038	1.407 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072318\
Data File : FG001750.D
Signal(s) : FID1A.ch
Acq On : 23 Jul 2018 14:32
Operator : AJ\SJ
Sample : J4081-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 24 05:05:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

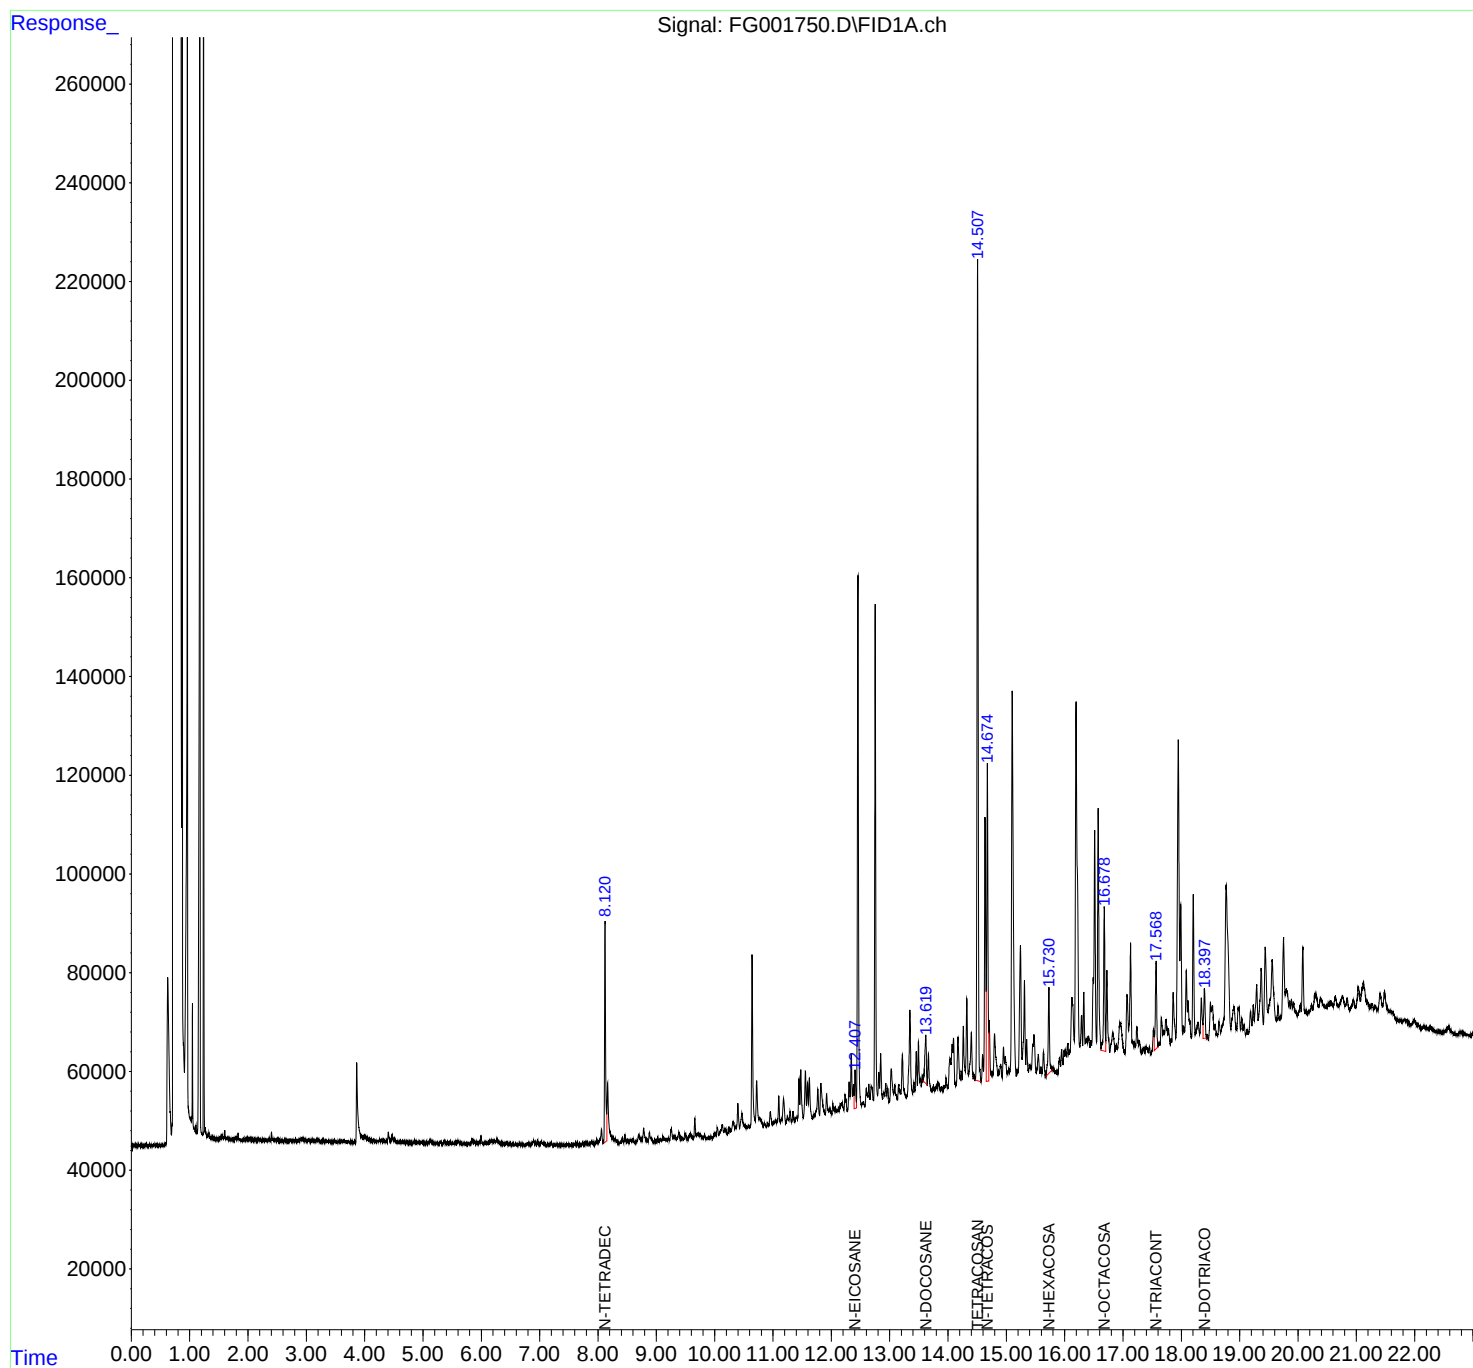


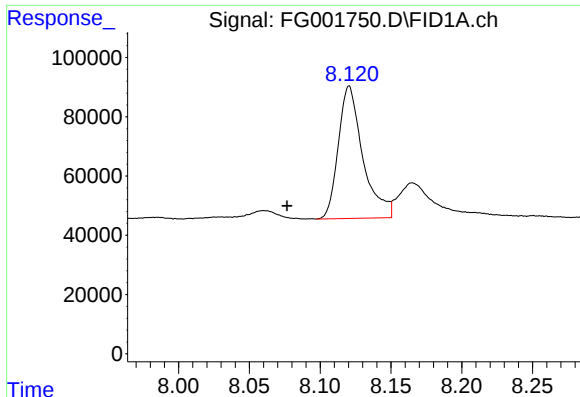

#4 N-TETRADECANE


R.T.: 8.120 min
Delta R.T.: 0.044 min
Response: 538373
Conc: 4.07 ug/ml

Instrument :
FID_G
ClientSampleId :

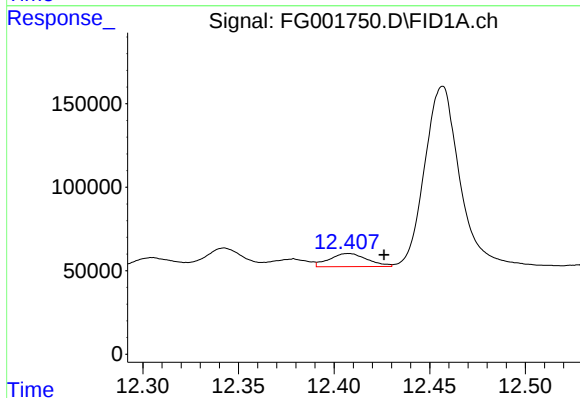


#7 N-EICOSANE

R.T.: 12.408 min
Delta R.T.: -0.019 min
Response: 107899
Conc: 0.81 ug/ml

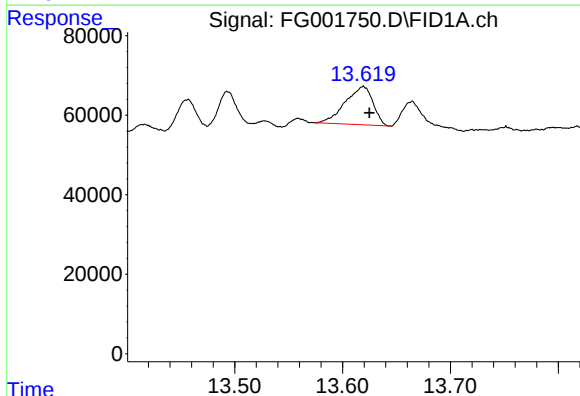


#8 N-DOCOSANE

R.T.: 13.619 min
Delta R.T.: -0.006 min
Response: 172087
Conc: 1.29 ug/ml

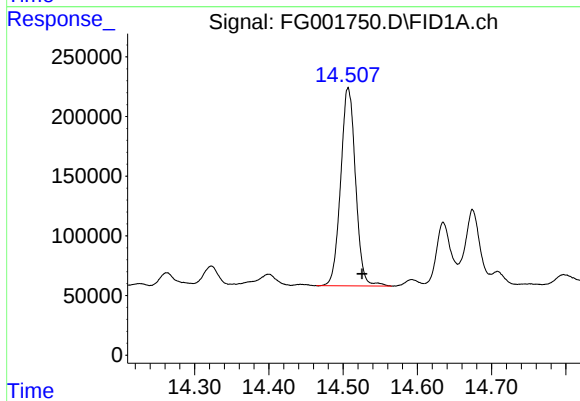

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.507 min
Delta R.T.: -0.019 min
Response: 2312094
Conc: 19.87 ug/ml

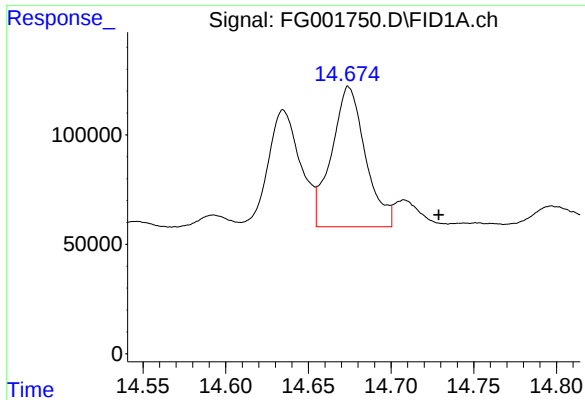

#10 N-TETRACOSANE


R.T.: 14.674 min
Delta R.T.: -0.054 min
Response: 913994
Conc: 6.91 ug/ml

Instrument :
FID_G
ClientSampleId :

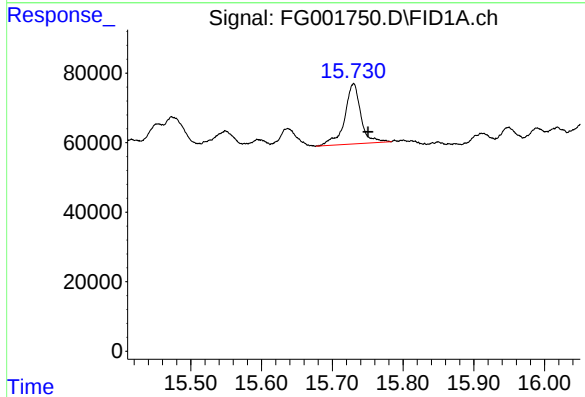


#11 N-HEXACOSANE

R.T.: 15.730 min
Delta R.T.: -0.020 min
Response: 274709
Conc: 2.09 ug/ml

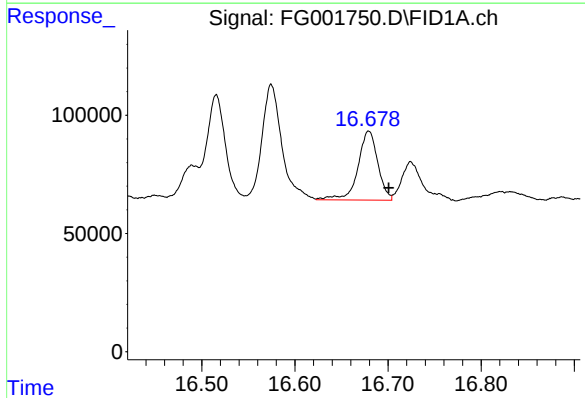


#12 N-OCTACOSANE

R.T.: 16.679 min
Delta R.T.: -0.021 min
Response: 432727
Conc: 3.31 ug/ml

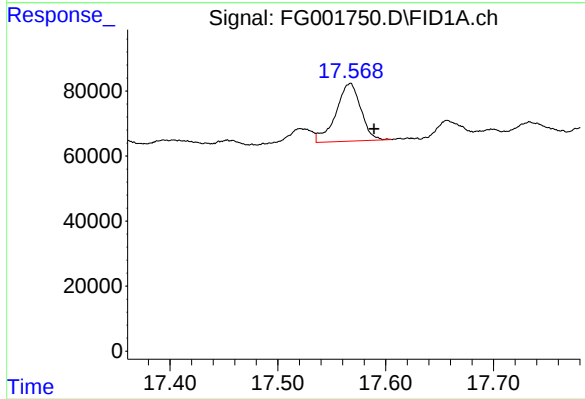

#13 N-TRIACONTANE

R.T.: 17.567 min
Delta R.T.: -0.022 min
Response: 284344
Conc: 2.18 ug/ml

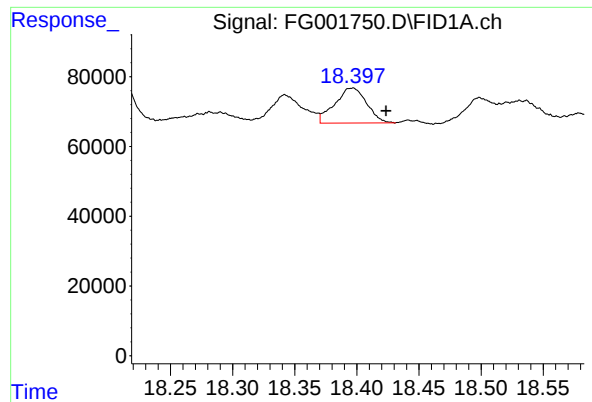

#14 N-DOTRIACONTANE

R.T.: 18.396 min
Delta R.T.: -0.027 min
Response: 179038
Conc: 1.41 ug/ml

Instrument :
FID_G
ClientSampleId :