

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072318\
 Data File : FG001746.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jul 2018 12:16
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 24 05:04:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.509	5737241	49.313 ug/ml
Target Compounds			
2) N-DECANE	4.252	6840778	53.023 ug/ml
3) N-DODECANE	6.270	6862438	52.170 ug/ml
4) N-TETRADECANE	8.063	6861276	51.875 ug/ml
5) N-HEXADECANE	9.662	6824334	51.600 ug/ml
6) N-OCTADECANE	11.102	6806021	50.886 ug/ml
7) N-EICOSANE	12.411	6697831	50.176 ug/ml
8) N-DOCOSANE	13.610	6597861	49.583 ug/ml
10) N-TETRACOSANE	14.713	6474940	48.977 ug/ml
11) N-HEXACOSANE	15.734	6357093	48.286 ug/ml
12) N-OCTACOSANE	16.683	6204038	47.456 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072318\
Data File : FG001746.D
Signal(s) : FID1A.ch
Acq On : 23 Jul 2018 12:16
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 24 05:04:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

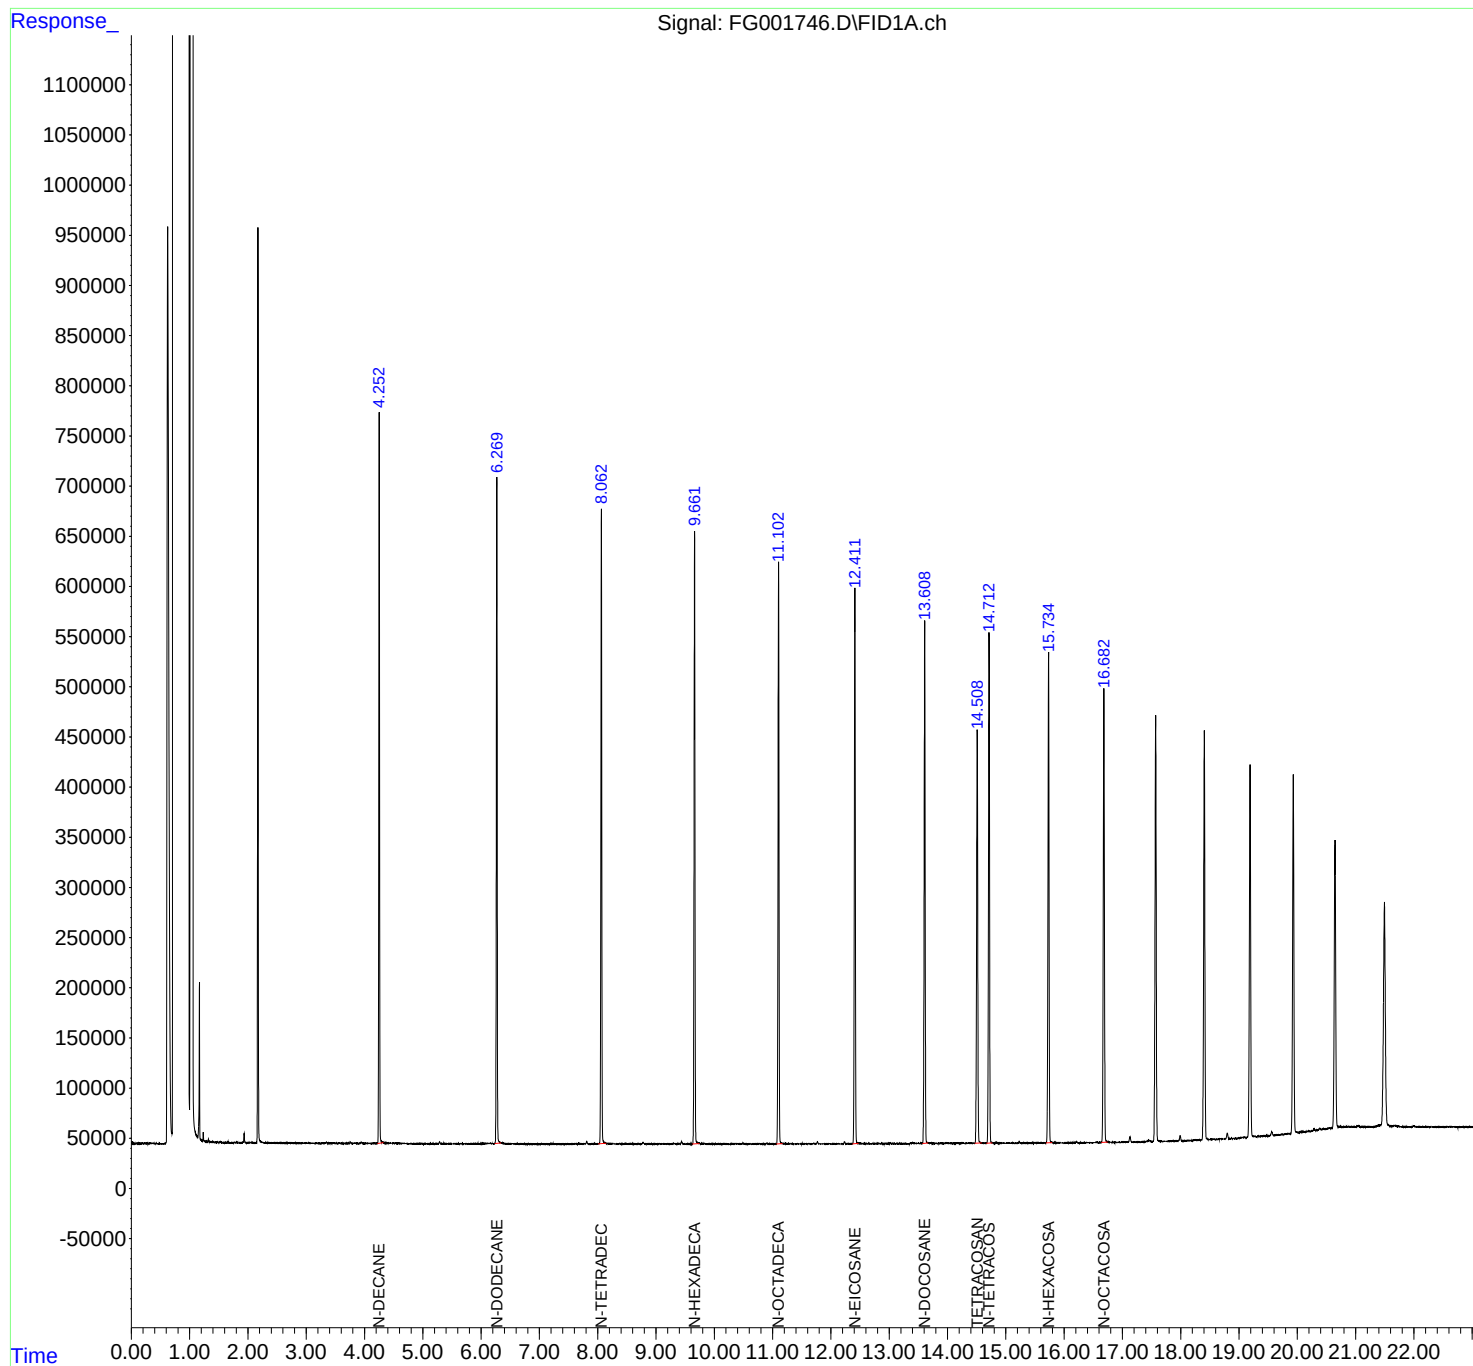


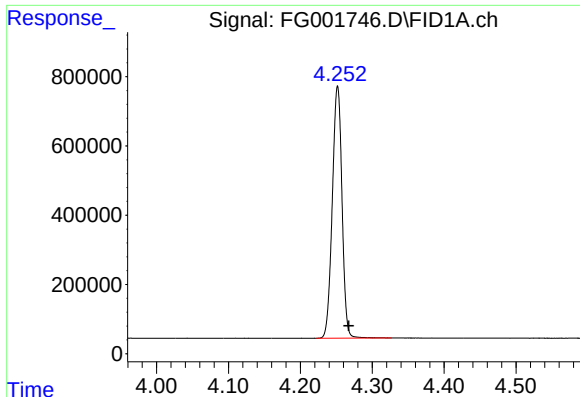

#2 N-DECANE


R.T.: 4.252 min
Delta R.T.: -0.016 min
Response: 6840778
Conc: 53.02 ug/ml

Instrument :
FID_G
ClientSampleId :

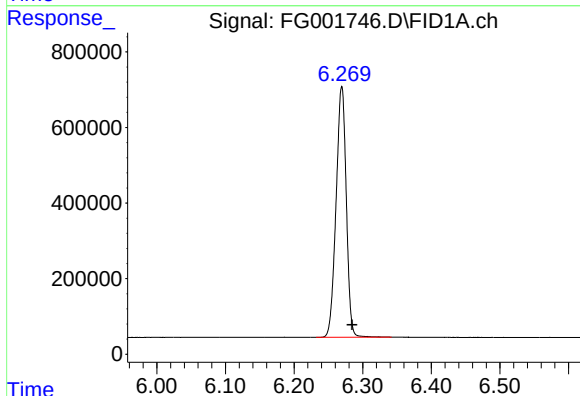


#3 N-DODECANE

R.T.: 6.270 min
Delta R.T.: -0.015 min
Response: 6862438
Conc: 52.17 ug/ml

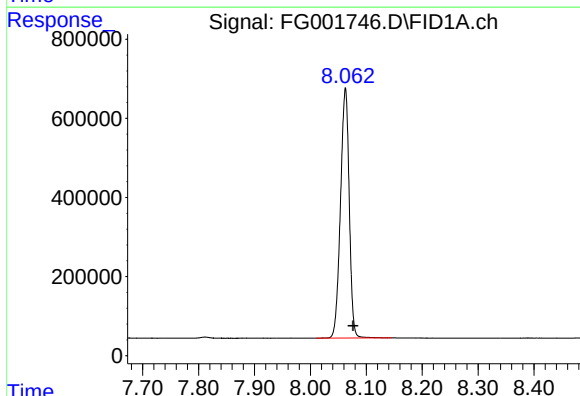


#4 N-TETRADECANE

R.T.: 8.063 min
Delta R.T.: -0.014 min
Response: 6861276
Conc: 51.88 ug/ml

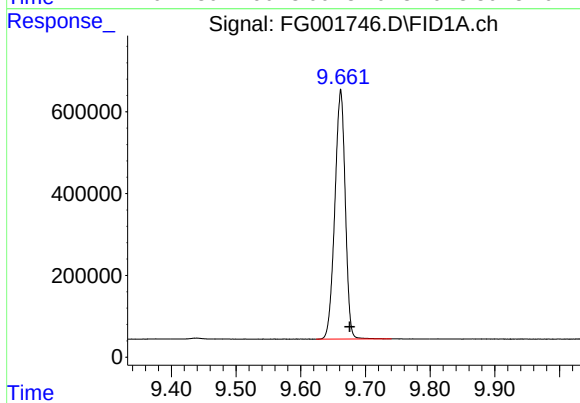

#5 N-HEXADECANE


R.T.: 9.662 min
Delta R.T.: -0.014 min
Response: 6824334
Conc: 51.60 ug/ml

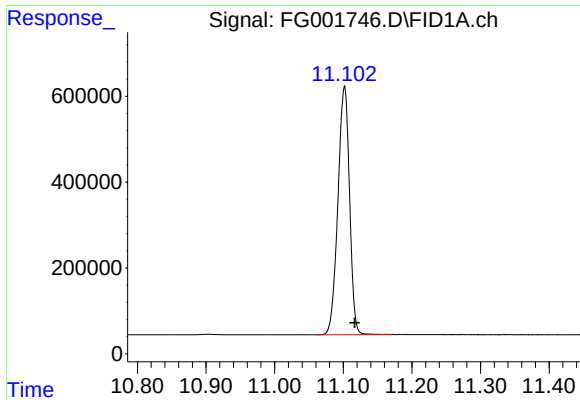

#6 N-OCTADECANE


R.T.: 11.102 min
Delta R.T.: -0.015 min
Response: 6806021
Conc: 50.89 ug/ml

Instrument :
FID_G
ClientSampleId :

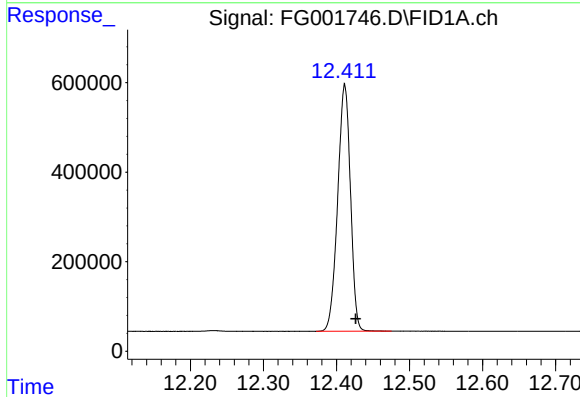


#7 N-EICOSANE

R.T.: 12.411 min
Delta R.T.: -0.015 min
Response: 6697831
Conc: 50.18 ug/ml

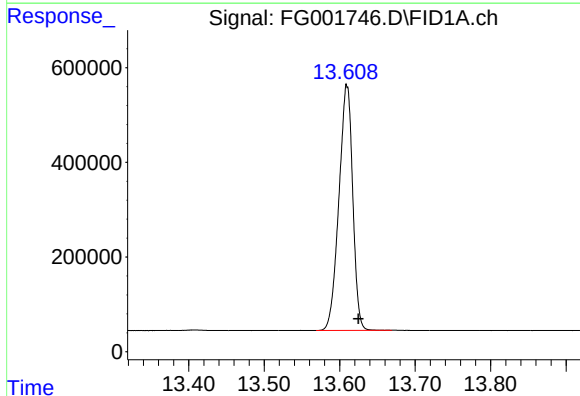


#8 N-DOCOSANE

R.T.: 13.610 min
Delta R.T.: -0.015 min
Response: 6597861
Conc: 49.58 ug/ml

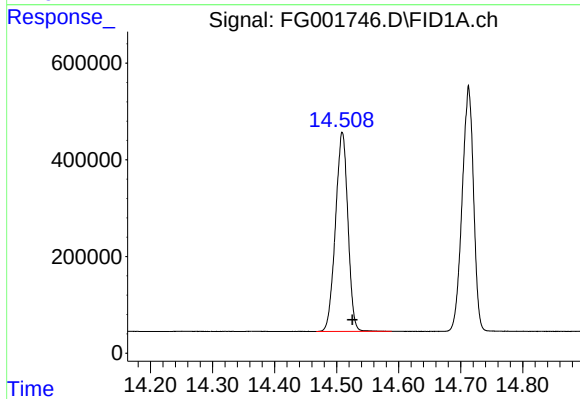

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.509 min
Delta R.T.: -0.016 min
Response: 5737241
Conc: 49.31 ug/ml

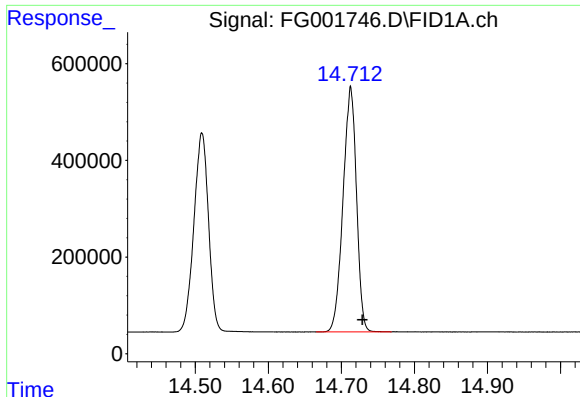

#10 N-TETRACOSANE


R.T.: 14.713 min
Delta R.T.: -0.016 min
Response: 6474940
Conc: 48.98 ug/ml

Instrument :
FID_G
ClientSampleId :

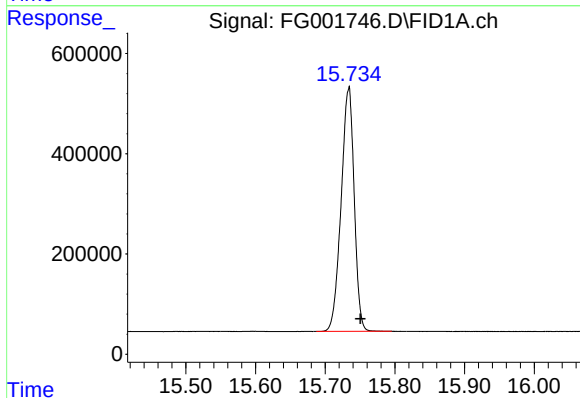

#11 N-HEXACOSANE

R.T.: 15.734 min
Delta R.T.: -0.017 min
Response: 6357093
Conc: 48.29 ug/ml

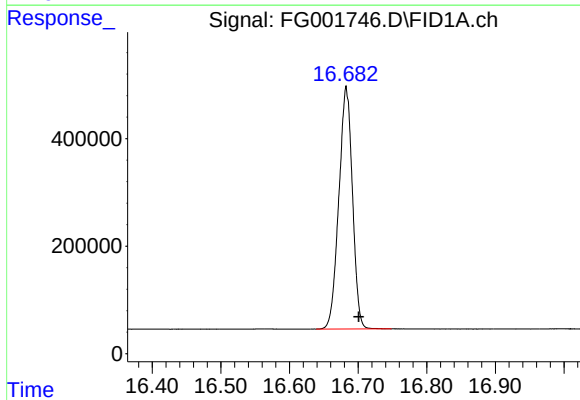

#12 N-OCTACOSANE

R.T.: 16.683 min
Delta R.T.: -0.018 min
Response: 6204038
Conc: 47.46 ug/ml