

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072420\
 Data File : FG007096.D
 Signal(s) : FID1A.ch
 Acq On : 24 Jul 2020 15:02
 Operator : DD\AJ
 Sample : L3394-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 25 01:02:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071520.M
 Quant Title :
 QLast Update : Thu Jul 16 02:29:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.784	2743407	16.781 ug/ml
Target Compounds			
4) N-TETRADECANE	8.284	319720	1.763 ug/ml
11) N-HEXACOSANE	16.011	148284	0.805 ug/ml
12) N-OCTACOSANE	16.962	349088	1.895 ug/ml
13) N-TRIACONTANE	17.852	478816	2.564 ug/ml
14) N-DOTRIACONTANE	18.682	445038	2.560 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072420\
Data File : FG007096.D
Signal(s) : FID1A.ch
Acq On : 24 Jul 2020 15:02
Operator : DD\AJ
Sample : L3394-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 25 01:02:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG071520.M
Quant Title :
QLast Update : Thu Jul 16 02:29:04 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

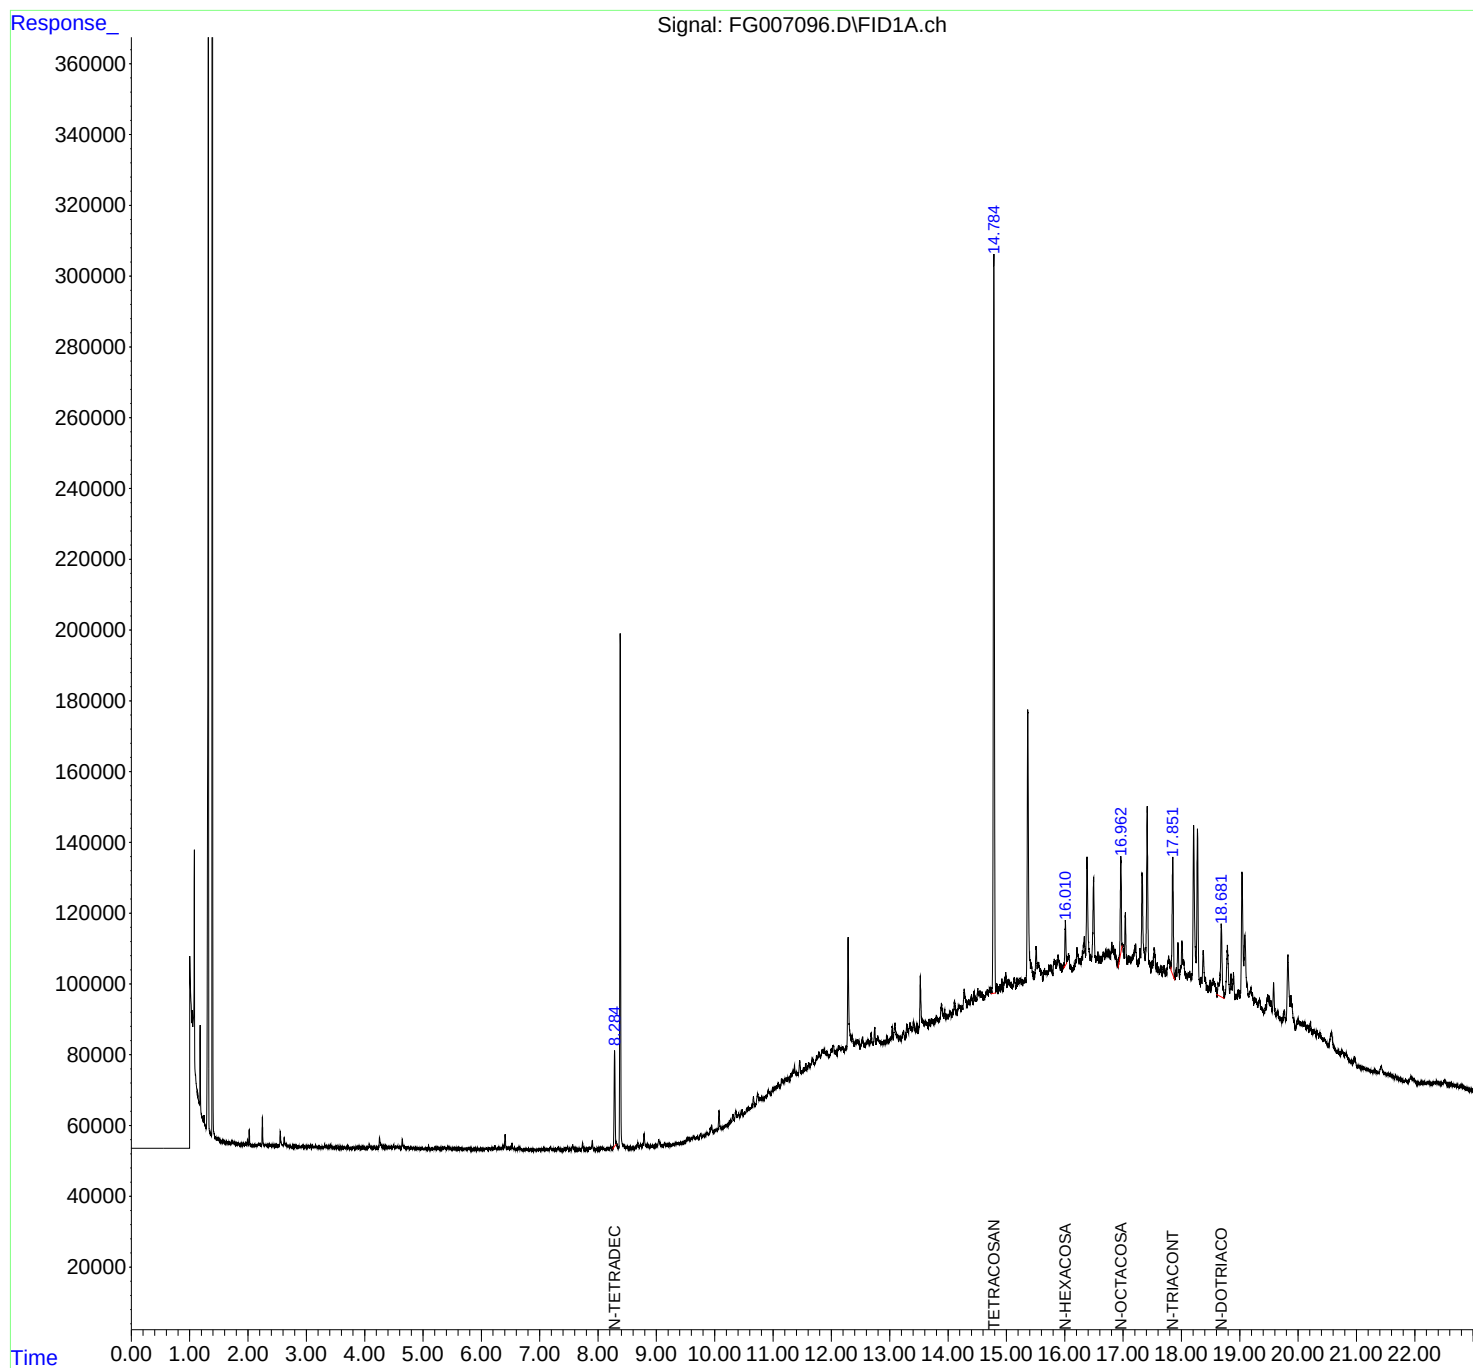


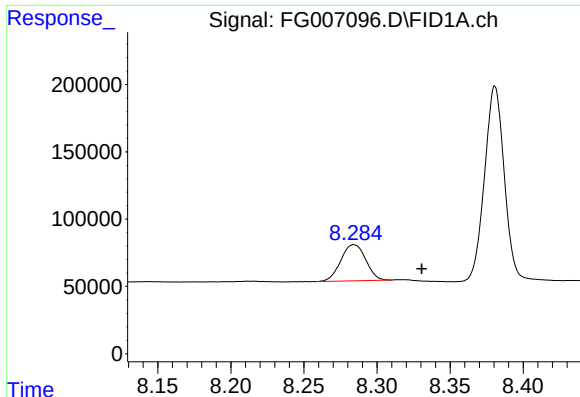

#4 N-TETRADECANE


R.T.: 8.284 min
Delta R.T.: -0.047 min
Response: 319720
Conc: 1.76 ug/ml

Instrument :
FID_G
ClientSampleId :

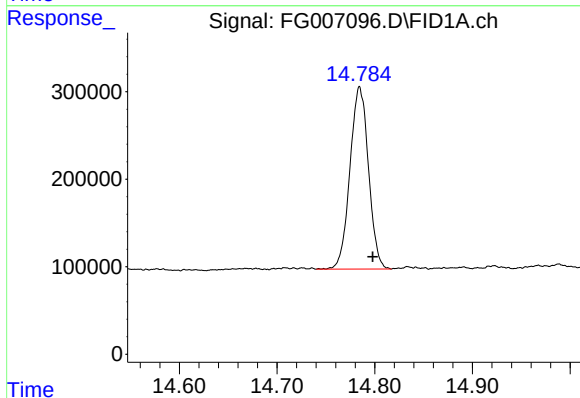


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.784 min
Delta R.T.: -0.013 min
Response: 2743407
Conc: 16.78 ug/ml

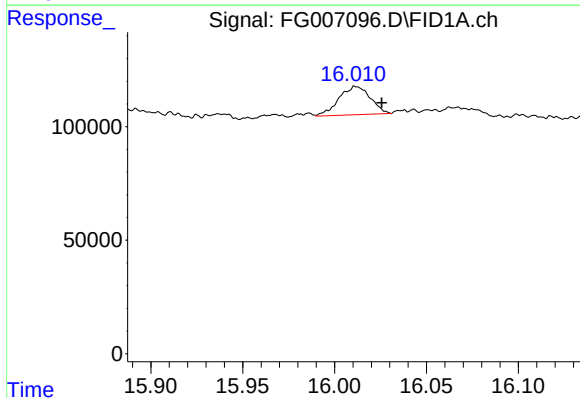


#11 N-HEXACOSANE

R.T.: 16.011 min
Delta R.T.: -0.014 min
Response: 148284
Conc: 0.80 ug/ml

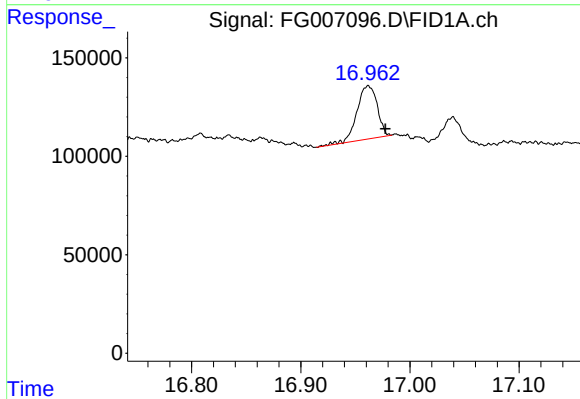

#12 N-OCTACOSANE


R.T.: 16.962 min
Delta R.T.: -0.016 min
Response: 349088
Conc: 1.90 ug/ml

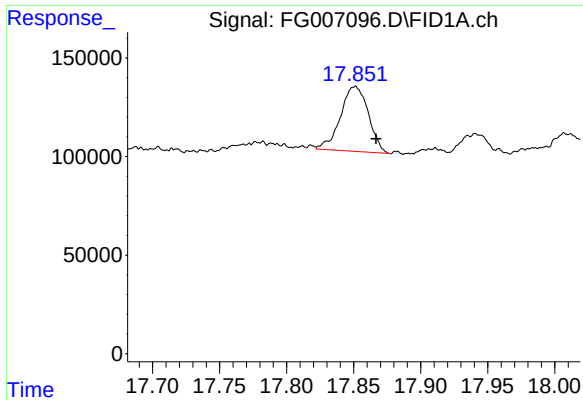

#13 N-TRIACONTANE

R.T.: 17.852 min
Delta R.T.: -0.015 min
Response: 478816
Conc: 2.56 ug/ml

Instrument :
FID_G
ClientSampleId :

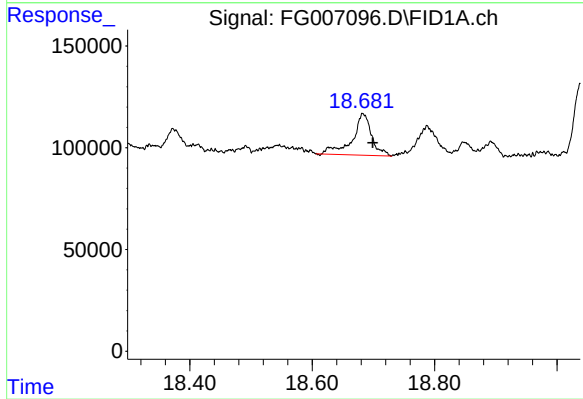

#14 N-DOTRIACONTANE

R.T.: 18.682 min
Delta R.T.: -0.017 min
Response: 445038
Conc: 2.56 ug/ml