

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072518\
 Data File : FG001793.D
 Signal(s) : FID1A.ch
 Acq On : 25 Jul 2018 16:55
 Operator : AJ\SJ
 Sample : J4124-06MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 26 08:38:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.505	1371524	11.789 ug/ml
Target Compounds				
2)	N-DECANE	4.253	1477087	11.449 ug/ml
3)	N-DODECANE	6.268	1500025	11.404 ug/ml
4)	N-TETRADECANE	8.060	1533463	11.594 ug/ml
5)	N-HEXADECANE	9.659	1533791	11.597 ug/ml
6)	N-OCTADECANE	11.099	1566913	11.715 ug/ml
7)	N-EICOSANE	12.407	1533290	11.487 ug/ml
8)	N-DOCOSANE	13.604	1533454	11.524 ug/ml
10)	N-TETRACOSANE	14.706	1594889	12.064 ug/mlm
11)	N-HEXACOSANE	15.729	1522012	11.561 ug/ml
12)	N-OCTACOSANE	16.679	1489774	11.396 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072518\
Data File : FG001793.D
Signal(s) : FID1A.ch
Acq On : 25 Jul 2018 16:55
Operator : AJ\SJ
Sample : J4124-06MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 26 08:38:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

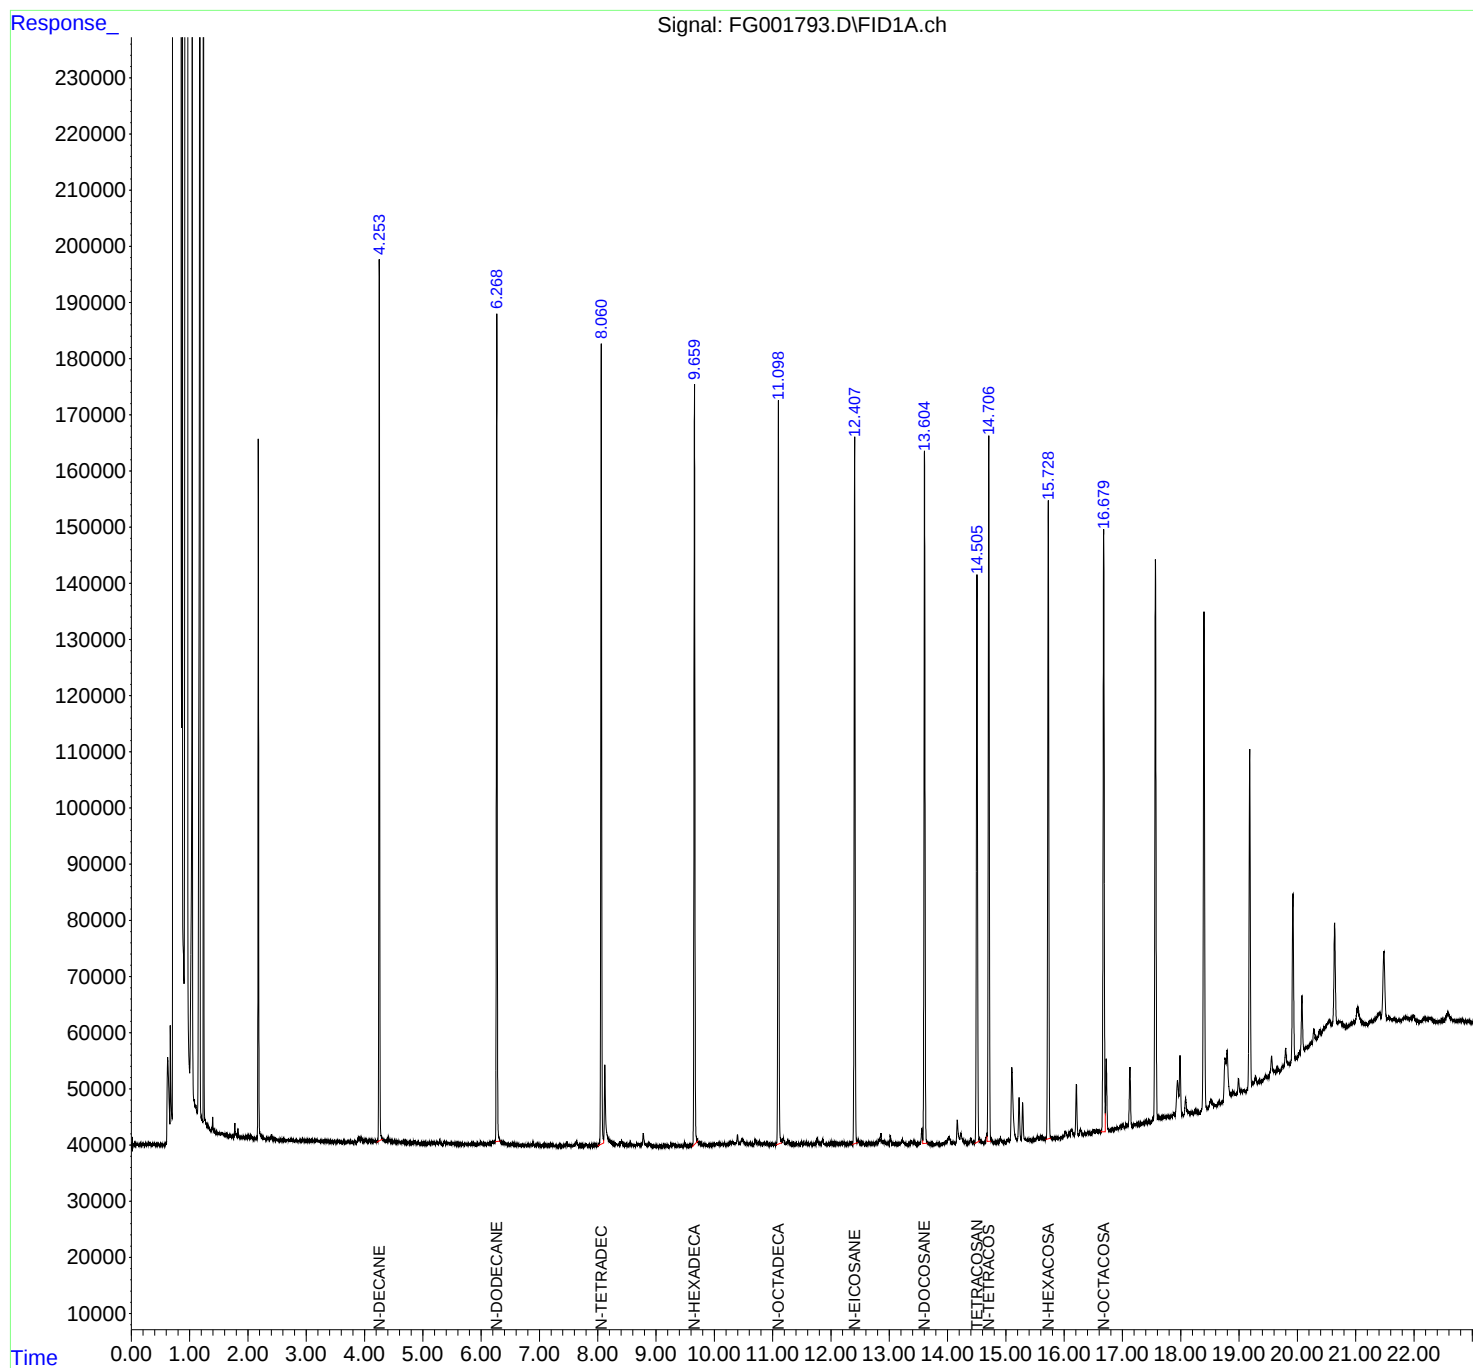

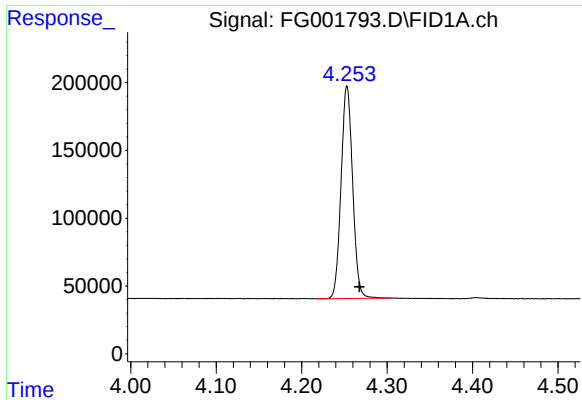


#2 N-DECANE

R.T.: 4.253 min
Delta R.T.: -0.014 min
Response: 1477087
Conc: 11.45 ug/ml

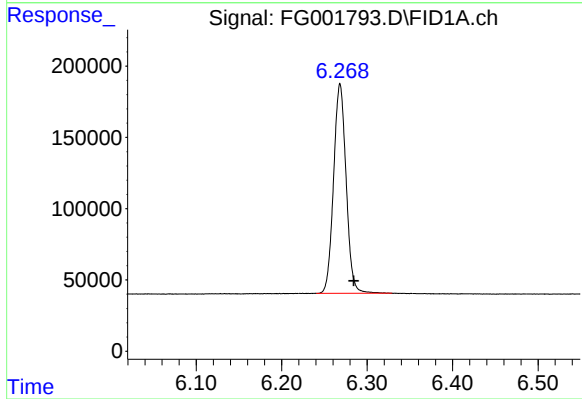


#3 N-DODECANE

R.T.: 6.268 min
Delta R.T.: -0.016 min
Response: 1500025
Conc: 11.40 ug/ml

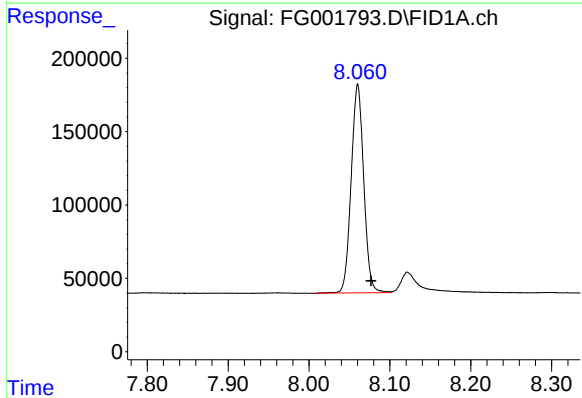


#4 N-TETRADECANE

R.T.: 8.060 min
Delta R.T.: -0.016 min
Response: 1533463
Conc: 11.59 ug/ml

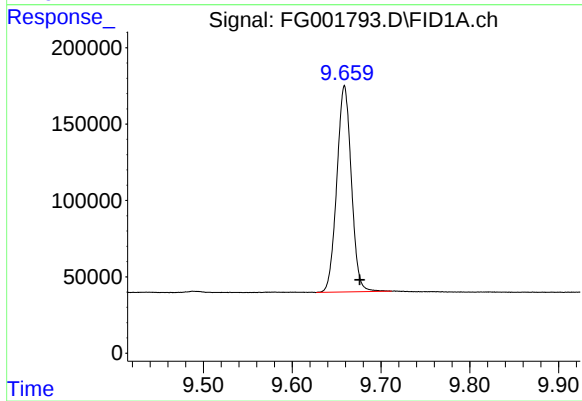


#5 N-HEXADECANE

R.T.: 9.659 min
Delta R.T.: -0.017 min
Response: 1533791
Conc: 11.60 ug/ml

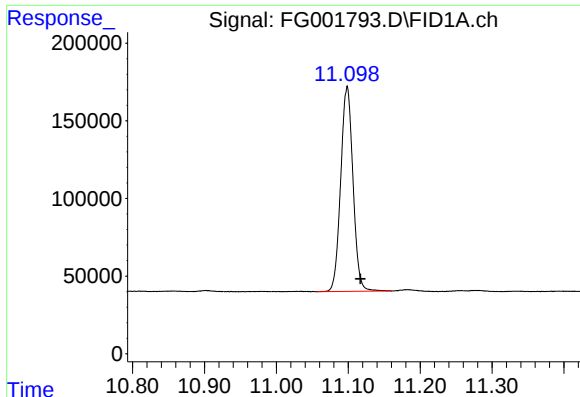


#6 N-OCTADECANE

R.T.: 11.099 min
Delta R.T.: -0.018 min
Response: 1566913
Conc: 11.72 ug/ml

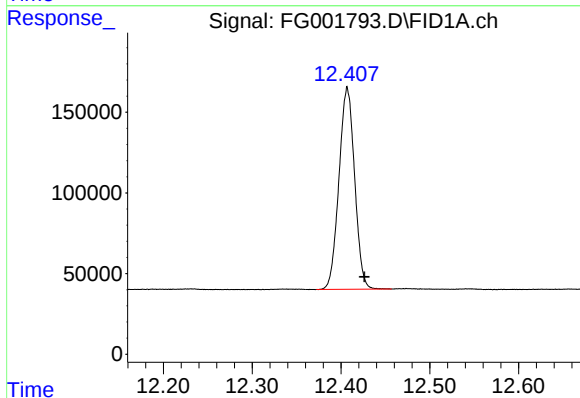


#7 N-EICOSANE

R.T.: 12.407 min
Delta R.T.: -0.019 min
Response: 1533290
Conc: 11.49 ug/ml

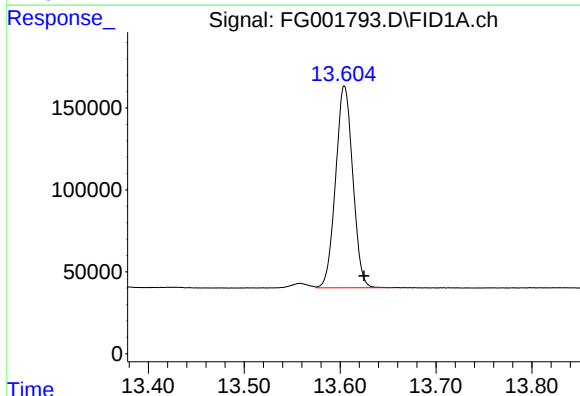


#8 N-DOCOSANE

R.T.: 13.604 min
Delta R.T.: -0.021 min
Response: 1533454
Conc: 11.52 ug/ml

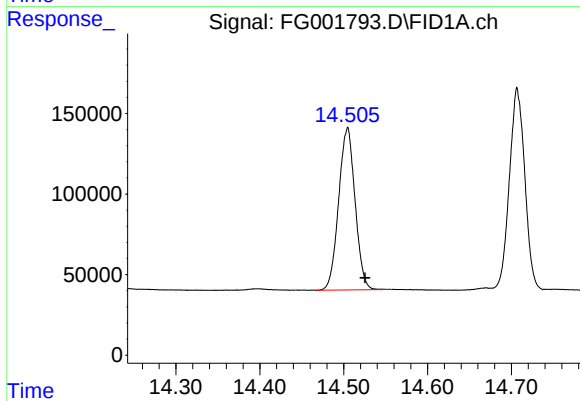


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.505 min
Delta R.T.: -0.021 min
Response: 1371524
Conc: 11.79 ug/ml

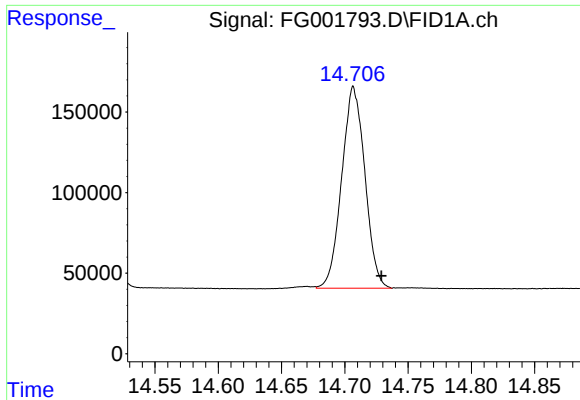


#10 N-TETRACOSANE

R.T.: 14.706 min
Delta R.T.: -0.023 min
Response: 1594889
Conc: 12.06 ug/ml m

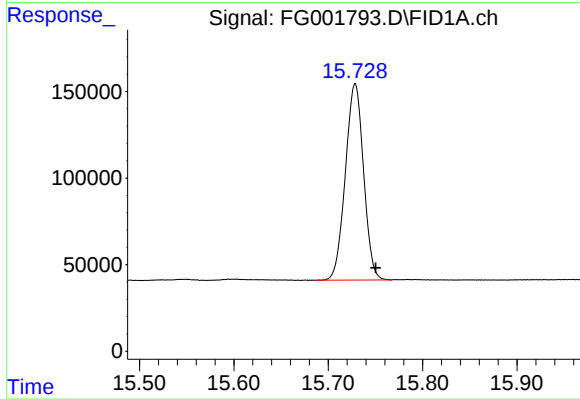

#11 N-HEXACOSANE

R.T.: 15.729 min
Delta R.T.: -0.022 min
Response: 1522012
Conc: 11.56 ug/ml

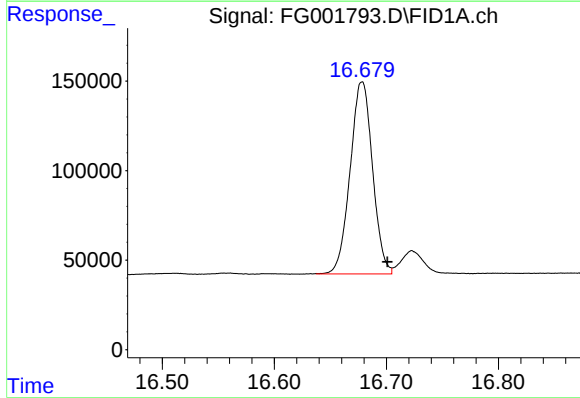

#12 N-OCTACOSANE

R.T.: 16.679 min
Delta R.T.: -0.022 min
Response: 1489774
Conc: 11.40 ug/ml m