

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001809.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 09:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 04:17:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.507	2899789	24.924 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.567	104227	0.800 ug/ml
14)	N-DOTRIACONTANE	18.400	156316	1.228 ug/ml
15)	N-TETRATRIACONTANE	19.184	88362	0.702 ug/ml
16)	N-HEXATRIACONTANE	19.927	63564	0.529 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001809.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 09:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 04:17:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

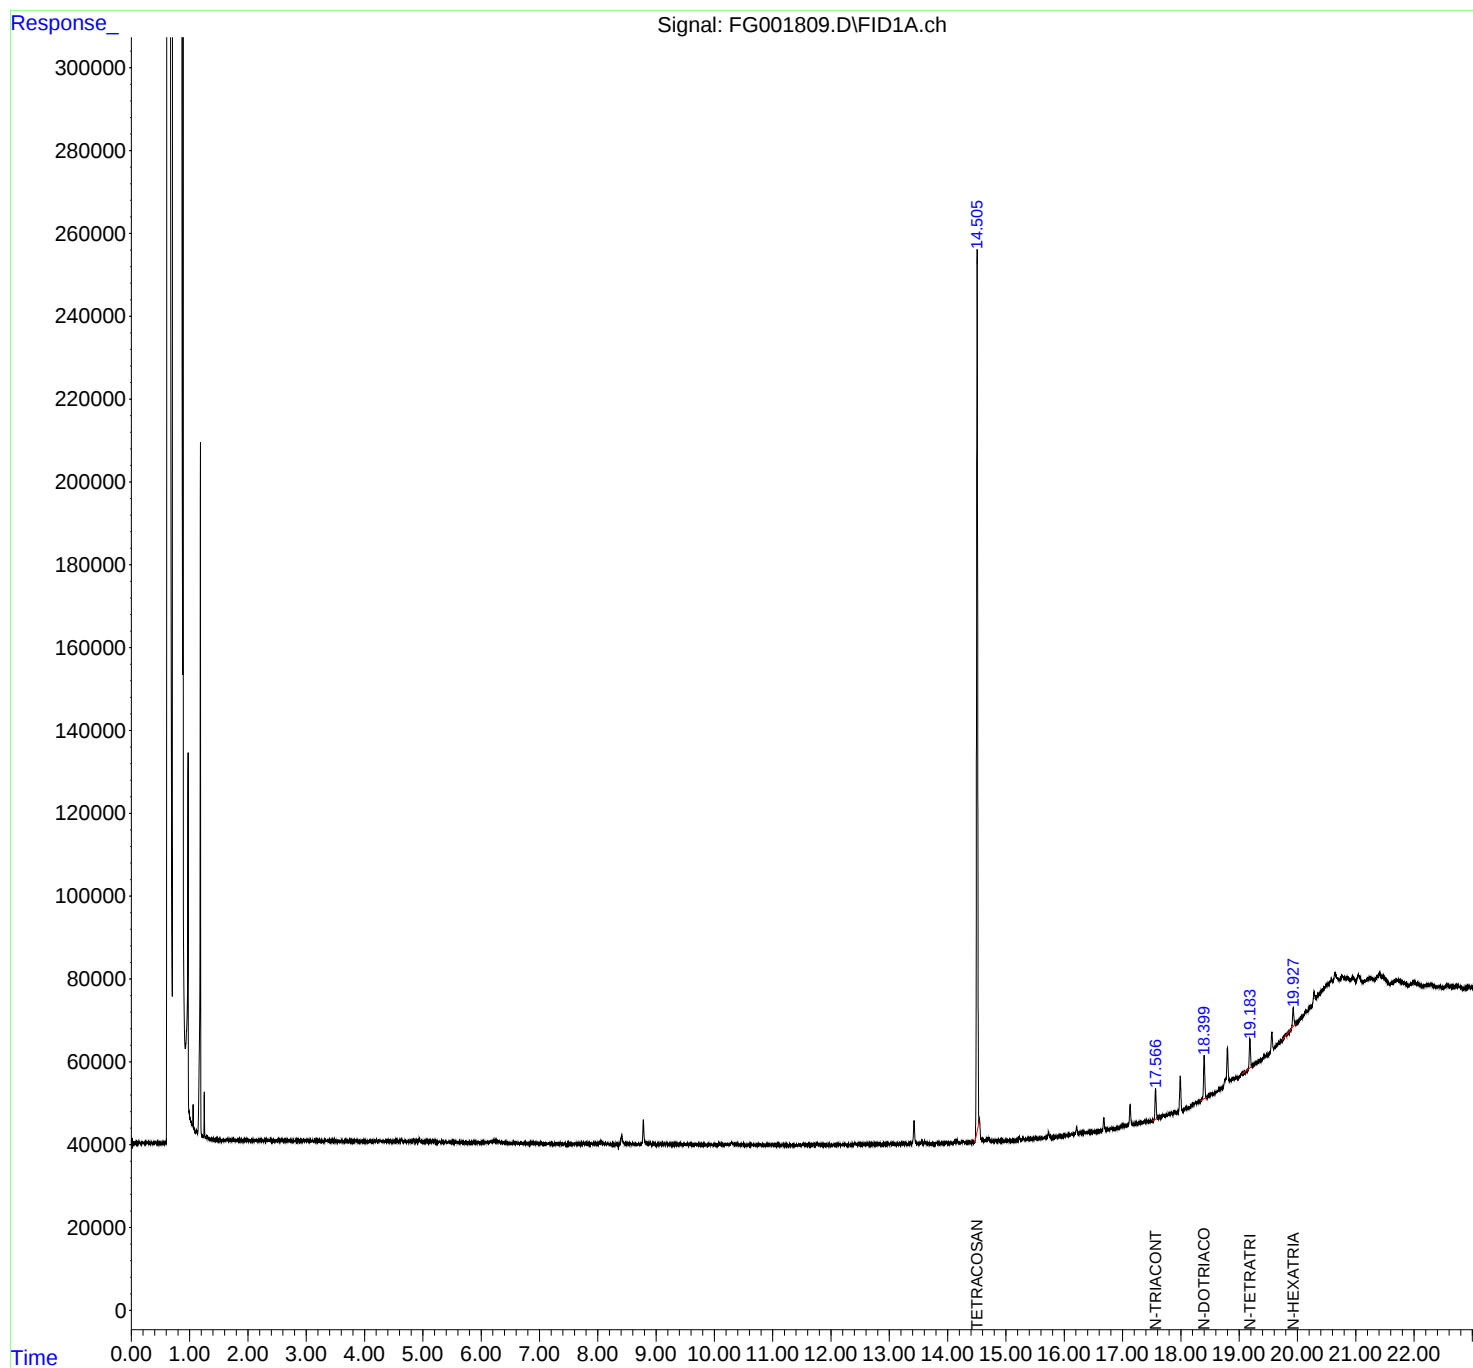


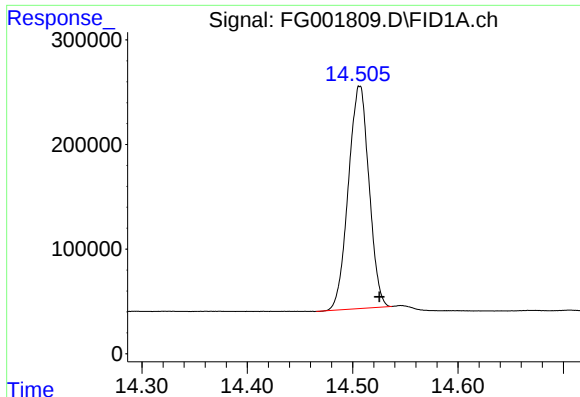

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.507 min
Delta R.T.: -0.019 min
Response: 2899789
Conc: 24.92 ug/ml

Instrument :
FID_G
ClientSampleId :

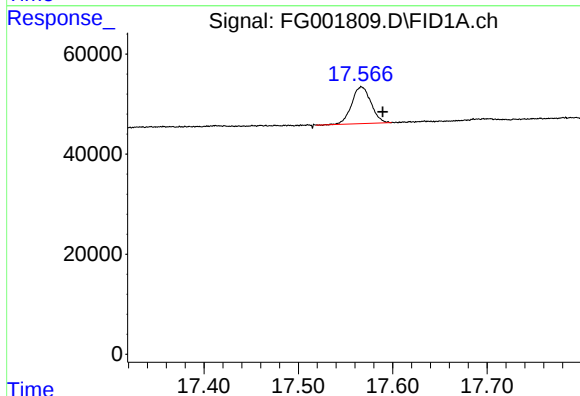


#13 N-TRIACONTANE

R.T.: 17.567 min
Delta R.T.: -0.022 min
Response: 104227
Conc: 0.80 ug/ml

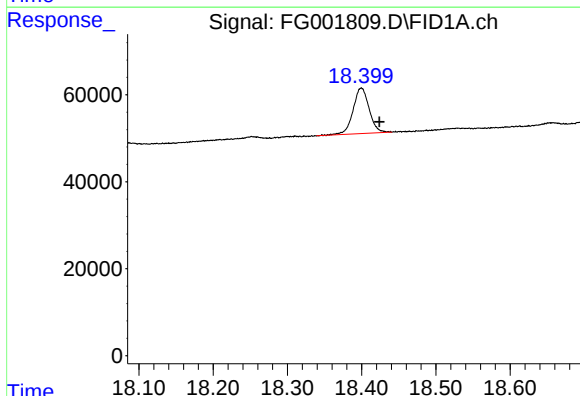


#14 N-DOTRIACONTANE

R.T.: 18.400 min
Delta R.T.: -0.024 min
Response: 156316
Conc: 1.23 ug/ml

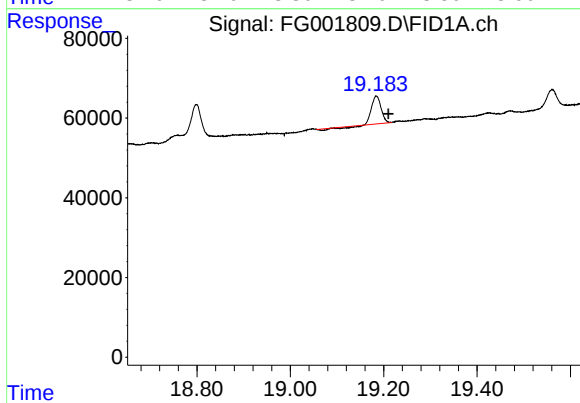

#15 N-TETRATRIACONTANE

R.T.: 19.184 min
Delta R.T.: -0.026 min
Response: 88362
Conc: 0.70 ug/ml

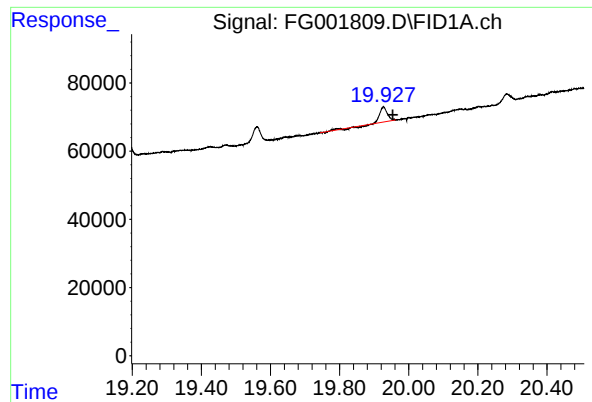

#16 N-HEXATRIACONTANE

R.T.: 19.927 min
Delta R.T.: -0.026 min
Response: 63564
Conc: 0.53 ug/ml

Instrument :
FID_G
ClientSampleId :