

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
 Data File : FG001812.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jul 2018 12:44
 Operator : AJ\SJ
 Sample : J4126-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 27 04:17:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.504	428090	3.680 ug/ml
Target Compounds			
4) N-TETRADECANE	8.112	100301	0.758 ug/ml
7) N-EICOSANE	12.402	140003	1.049 ug/ml
8) N-DOCOSANE	13.616	329967	2.480 ug/ml
10) N-TETRACOSANE	14.756	686774	5.195 ug/ml
12) N-OCTACOSANE	16.678	514898	3.939 ug/ml
13) N-TRIACONTANE	17.570	307934	2.364 ug/ml
14) N-DOTRIACONTANE	18.402	154733	1.216 ug/ml
15) N-TETRATRIACONTANE	19.193	226871	1.803 ug/ml
16) N-HEXATRIACONTANE	19.895f	230201	1.916 ug/ml
18) N-TETRACONTANE	21.488	134329	1.288 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001812.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 12:44
Operator : AJ\SJ
Sample : J4126-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 04:17:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

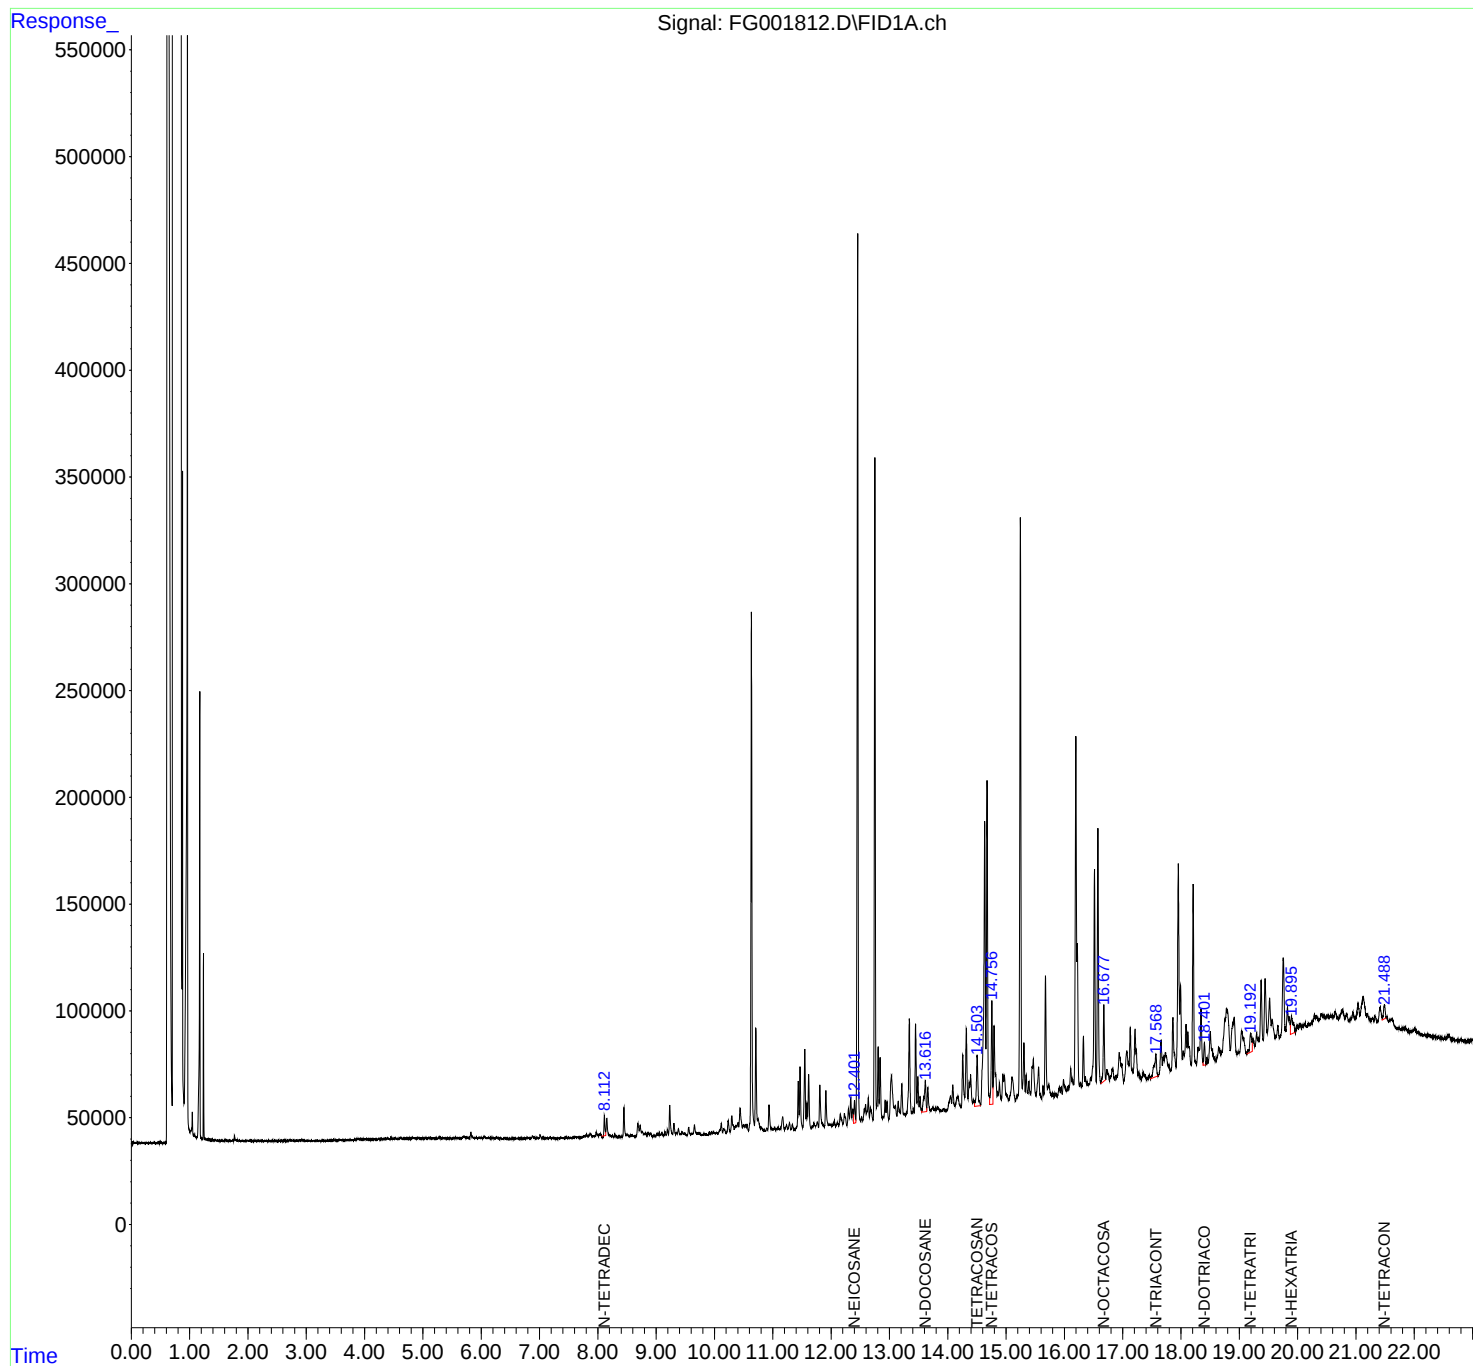


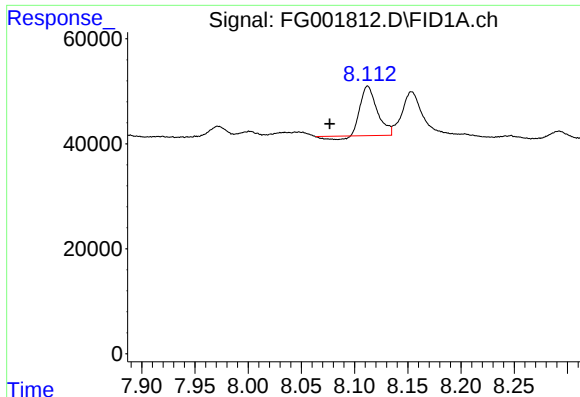

#4 N-TETRADECANE


R.T.: 8.112 min
Delta R.T.: 0.036 min
Response: 100301
Conc: 0.76 ug/ml

Instrument :
FID_G
ClientSampleId :

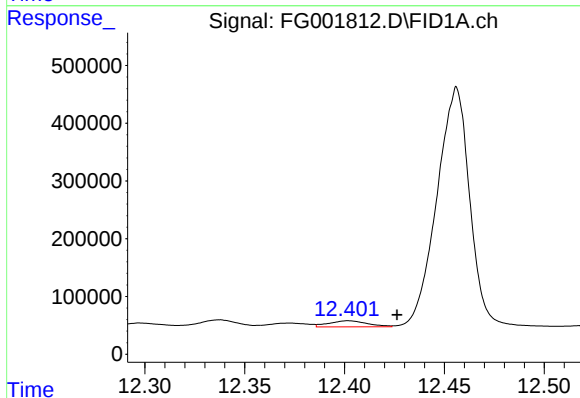


#7 N-EICOSANE

R.T.: 12.402 min
Delta R.T.: -0.024 min
Response: 140003
Conc: 1.05 ug/ml

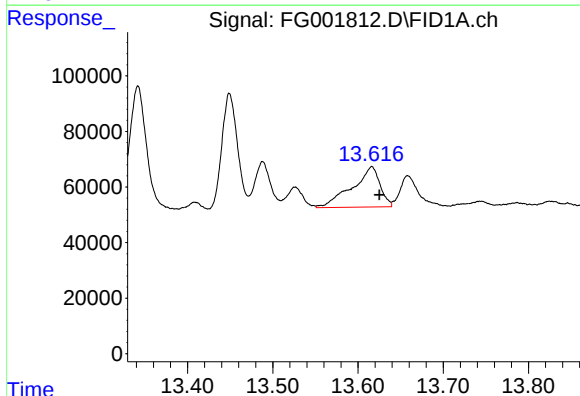


#8 N-DOCOSANE

R.T.: 13.616 min
Delta R.T.: -0.009 min
Response: 329967
Conc: 2.48 ug/ml

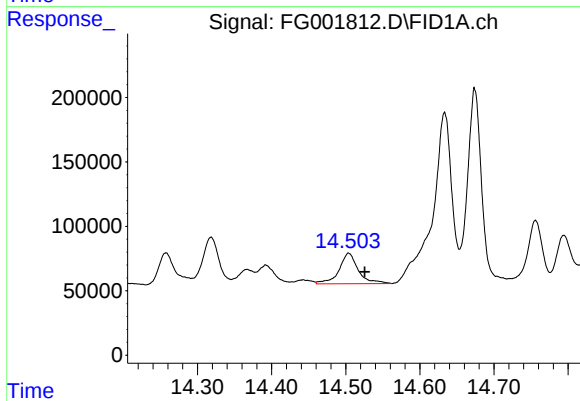

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.504 min
Delta R.T.: -0.021 min
Response: 428090
Conc: 3.68 ug/ml

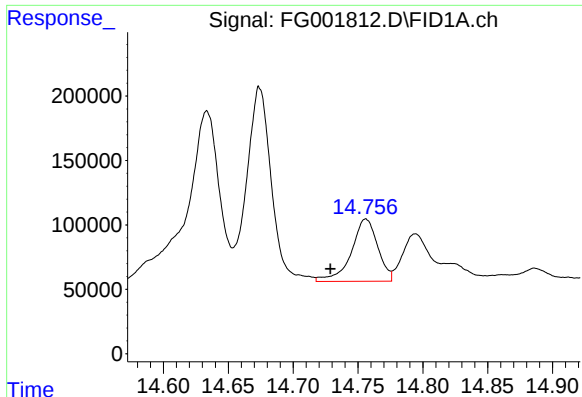

#10 N-TETRACOSANE


R.T.: 14.756 min
Delta R.T.: 0.027 min
Response: 686774
Conc: 5.19 ug/ml

Instrument :
FID_G
ClientSampleId :

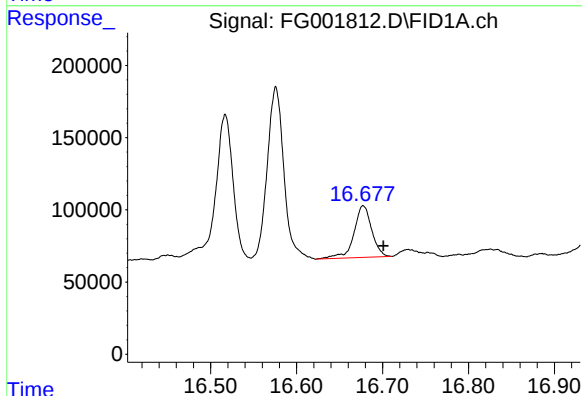


#12 N-OCTACOSANE

R.T.: 16.678 min
Delta R.T.: -0.023 min
Response: 514898
Conc: 3.94 ug/ml

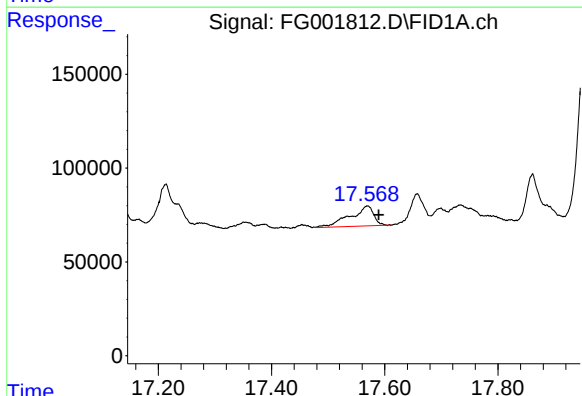


#13 N-TRIACONTANE

R.T.: 17.570 min
Delta R.T.: -0.020 min
Response: 307934
Conc: 2.36 ug/ml

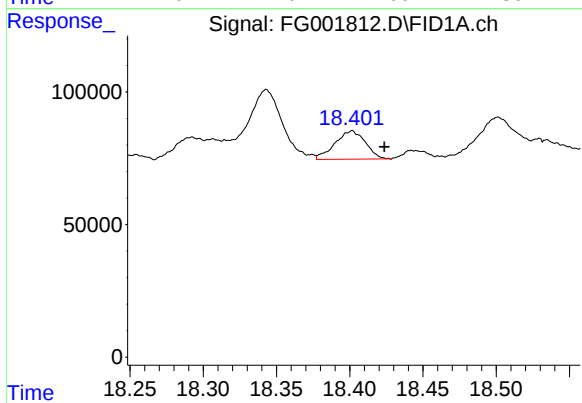

#14 N-DOTRIACONTANE


R.T.: 18.402 min
Delta R.T.: -0.022 min
Response: 154733
Conc: 1.22 ug/ml

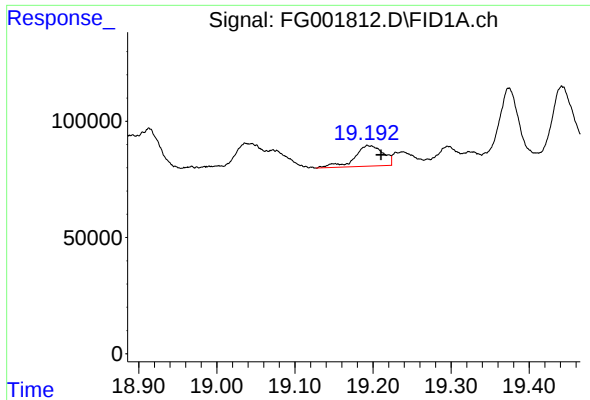

#15 N-TETRATRIACONTANE


R.T.: 19.193 min
Delta R.T.: -0.017 min
Response: 226871
Conc: 1.80 ug/ml

Instrument :
FID_G
ClientSampleId :

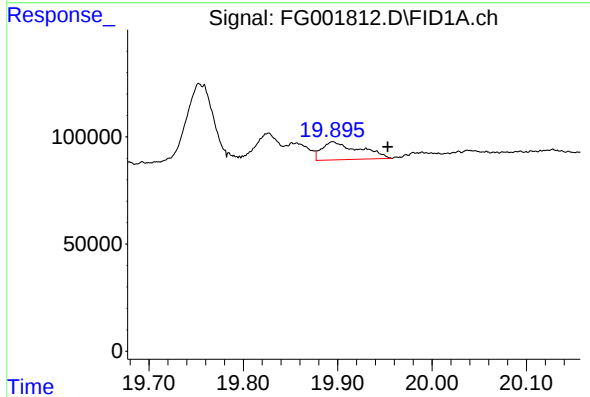

#16 N-HEXATRIACONTANE

R.T.: 19.895 min
Delta R.T.: -0.058 min
Response: 230201
Conc: 1.92 ug/ml

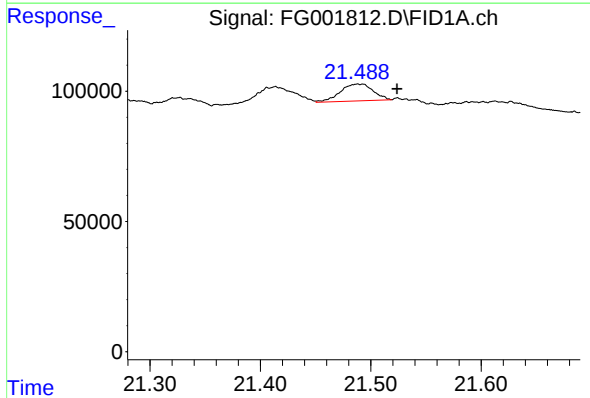

#18 N-TETRACONTANE

R.T.: 21.488 min
Delta R.T.: -0.036 min
Response: 134329
Conc: 1.29 ug/ml