

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
 Data File : FG001816.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jul 2018 15:11
 Operator : AJ\SJ
 Sample : J4126-11 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 27 04:18:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.505	322900	2.775 ug/ml
Target Compounds			
4) N-TETRADECANE	8.038	143806	1.087 ug/ml
6) N-OCTADECANE	11.175f	414072	3.096 ug/ml
7) N-EICOSANE	12.404	155774	1.167 ug/ml
8) N-DOCOSANE	13.619	352540	2.649 ug/ml
10) N-TETRACOSANE	14.675f	1507918	11.406 ug/ml
12) N-OCTACOSANE	16.677	297147	2.273 ug/ml
13) N-TRIACONTANE	17.569	163713	1.257 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001816.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 15:11
Operator : AJ\SJ
Sample : J4126-11 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 04:18:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

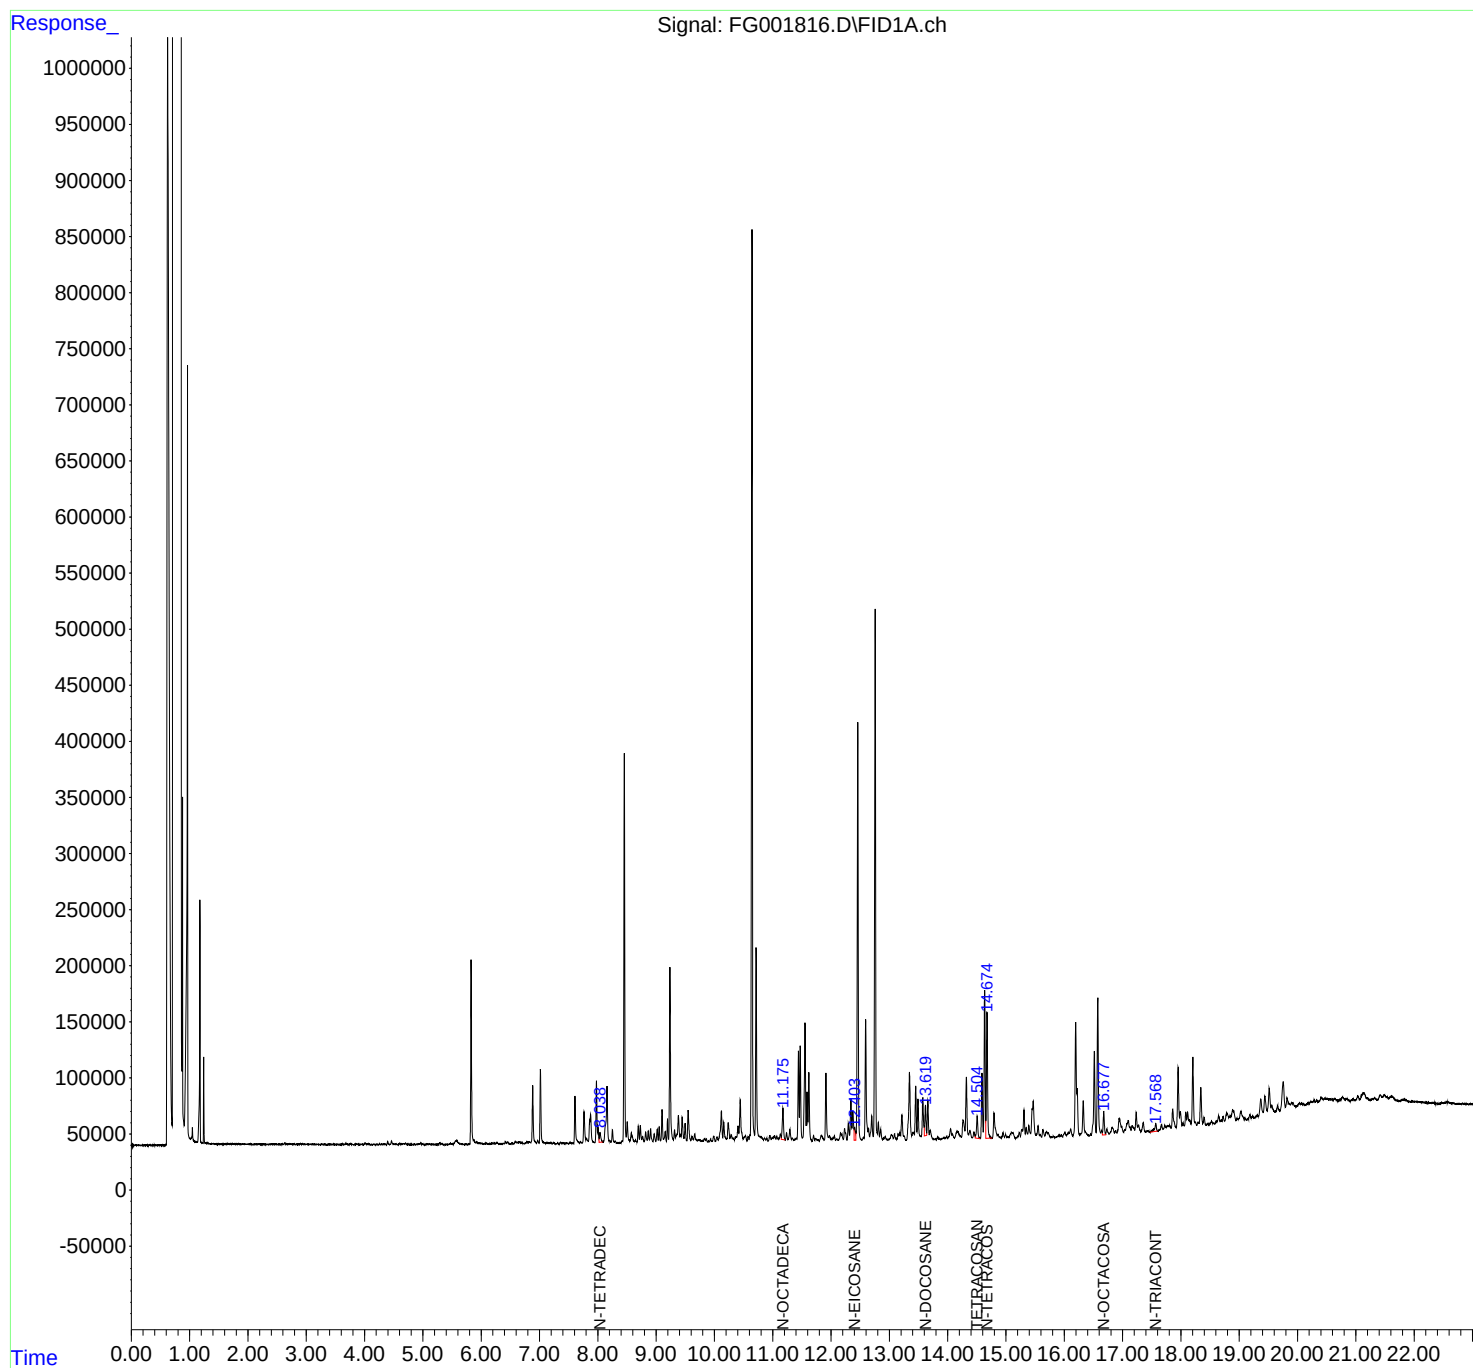


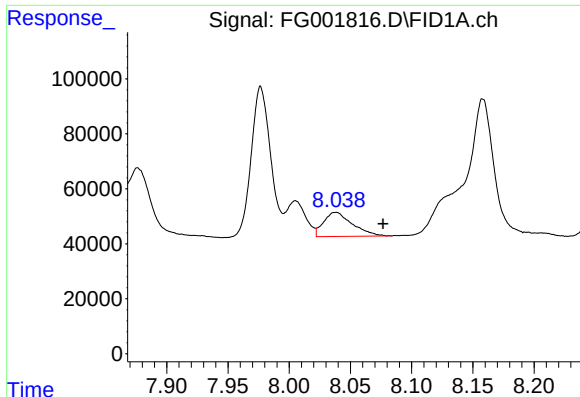

#4 N-TETRADECANE


R.T.: 8.038 min
Delta R.T.: -0.039 min
Response: 143806
Conc: 1.09 ug/ml

Instrument :
FID_G
ClientSampleId :

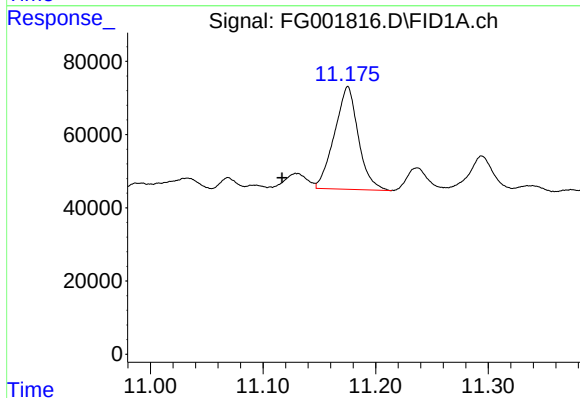


#6 N-OCTADECANE

R.T.: 11.175 min
Delta R.T.: 0.058 min
Response: 414072
Conc: 3.10 ug/ml

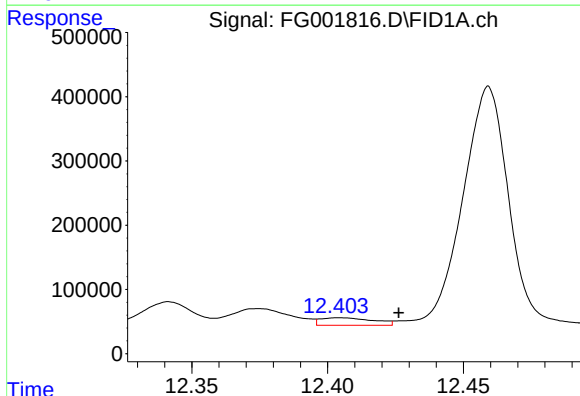


#7 N-EICOSANE

R.T.: 12.404 min
Delta R.T.: -0.022 min
Response: 155774
Conc: 1.17 ug/ml

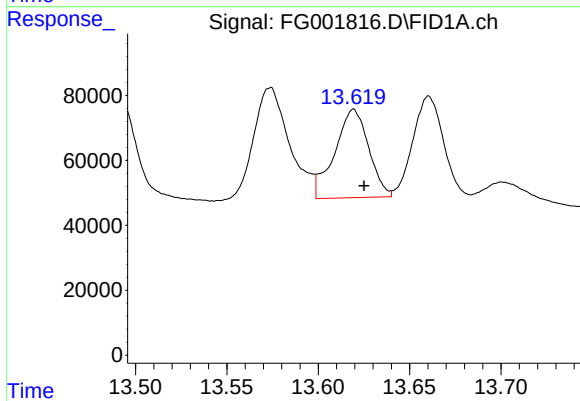

#8 N-DOCOSANE


R.T.: 13.619 min
Delta R.T.: -0.006 min
Response: 352540
Conc: 2.65 ug/ml

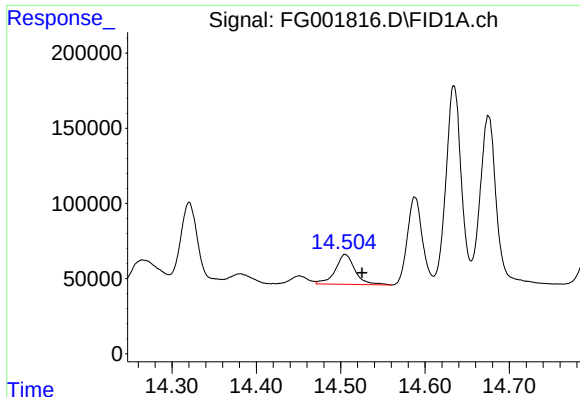

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.505 min
Delta R.T.: -0.020 min
Response: 322900
Conc: 2.78 ug/ml

Instrument :
FID_G
ClientSampleId :

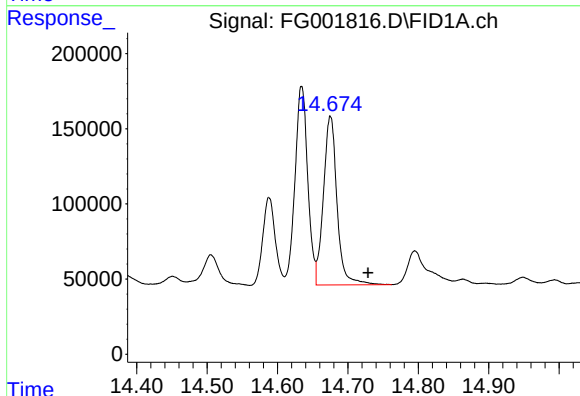


#10 N-TETRACOSANE

R.T.: 14.675 min
Delta R.T.: -0.054 min
Response: 1507918
Conc: 11.41 ug/ml

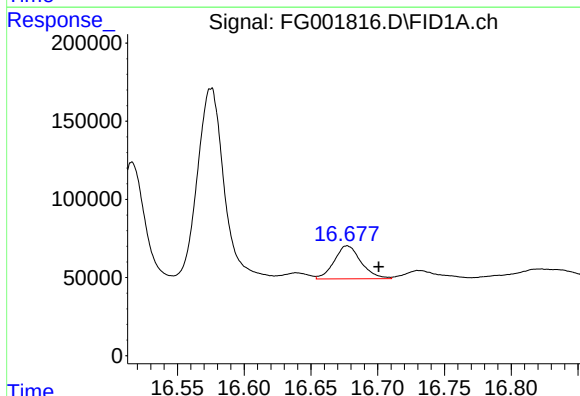

#12 N-OCTACOSANE

R.T.: 16.677 min
Delta R.T.: -0.024 min
Response: 297147
Conc: 2.27 ug/ml

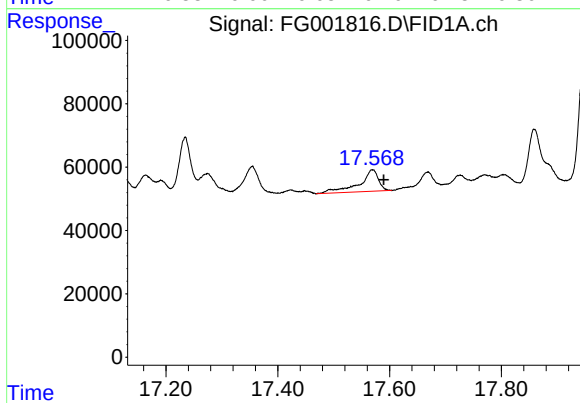

#13 N-TRIACONTANE

R.T.: 17.569 min
Delta R.T.: -0.020 min
Response: 163713
Conc: 1.26 ug/ml