

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001818.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 16:11
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 04:18:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.507	2912866	25.037 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.567	129717	0.996 ug/ml
14) N-DOTRIACONTANE	18.400	183587	1.442 ug/ml
15) N-TETRATRIACONTANE	19.186	116374	0.925 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001818.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 16:11
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 04:18:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

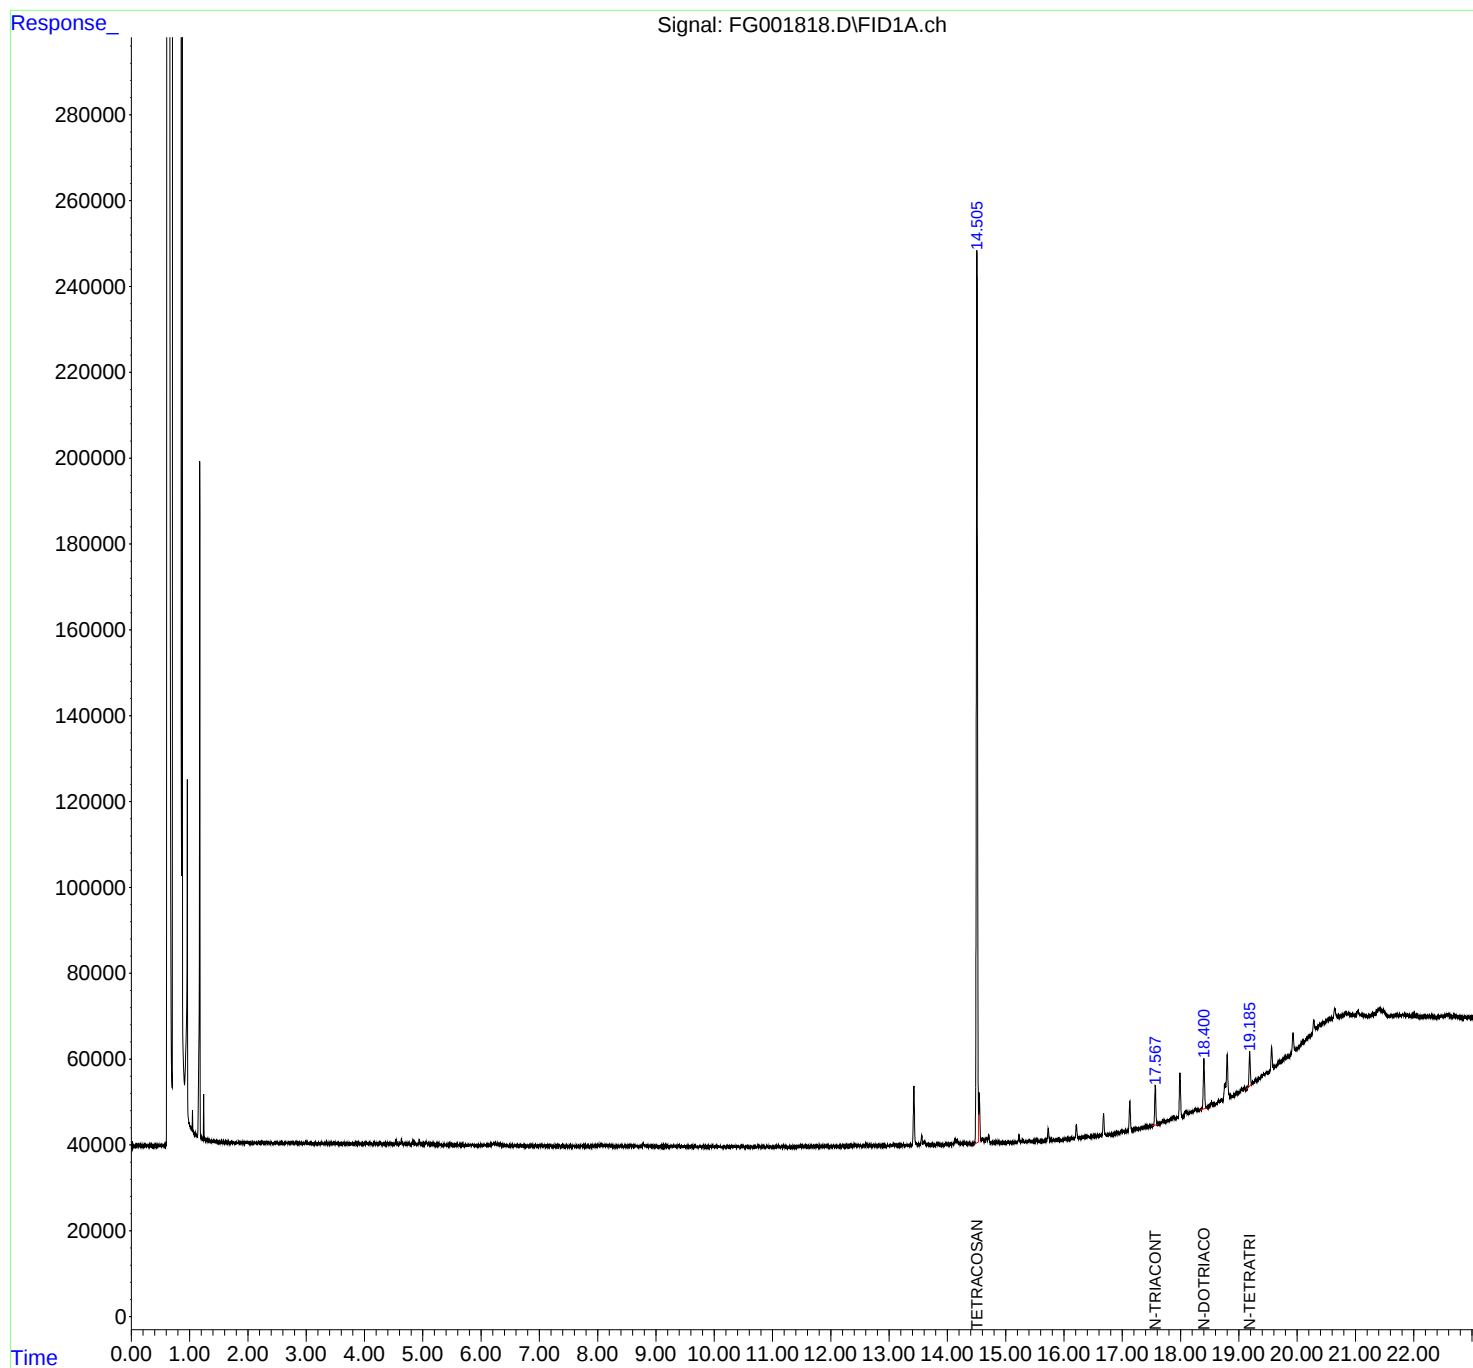


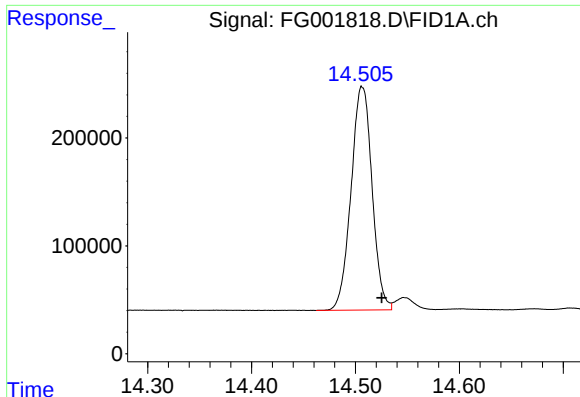

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.507 min
Delta R.T.: -0.019 min
Response: 2912866
Conc: 25.04 ug/ml

Instrument :
FID_G
ClientSampleId :

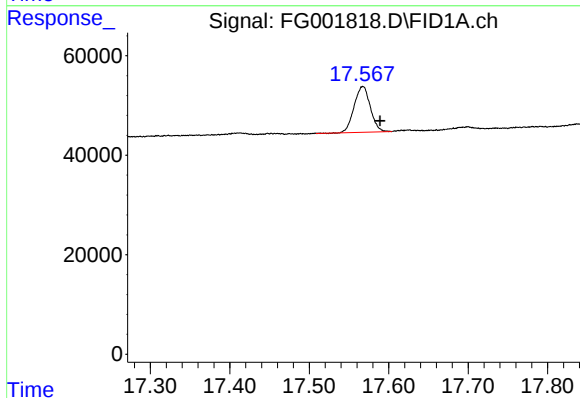


#13 N-TRIACONTANE

R.T.: 17.567 min
Delta R.T.: -0.022 min
Response: 129717
Conc: 1.00 ug/ml

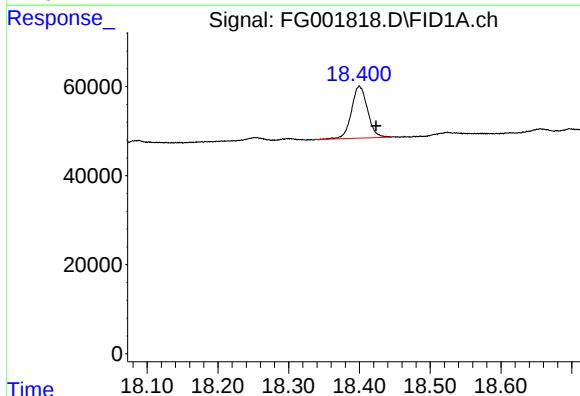

#14 N-DOTRIACONTANE

R.T.: 18.400 min
Delta R.T.: -0.024 min
Response: 183587
Conc: 1.44 ug/ml

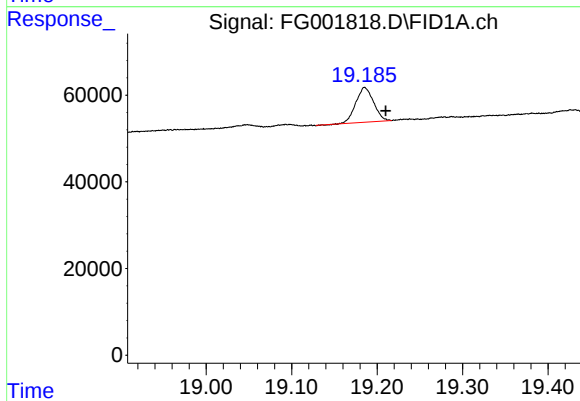

#15 N-TETRATRIACONTANE

R.T.: 19.186 min
Delta R.T.: -0.025 min
Response: 116374
Conc: 0.92 ug/ml