

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001816.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 15:11
Operator : AJ\SJ
Sample : J4126-11 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
2018-NYSEG-CLARK-AREA-8

Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:00 AM

Integration File: autoint1.e
Quant Time: Jul 27 04:18:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.504	295666	2.541 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001816.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 15:11
Operator : AJ\SJ
Sample : J4126-11 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
2018-NYSEG-CLARK-AREA-8


Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:00 AM

Integration File: autoint1.e
Quant Time: Jul 27 04:18:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

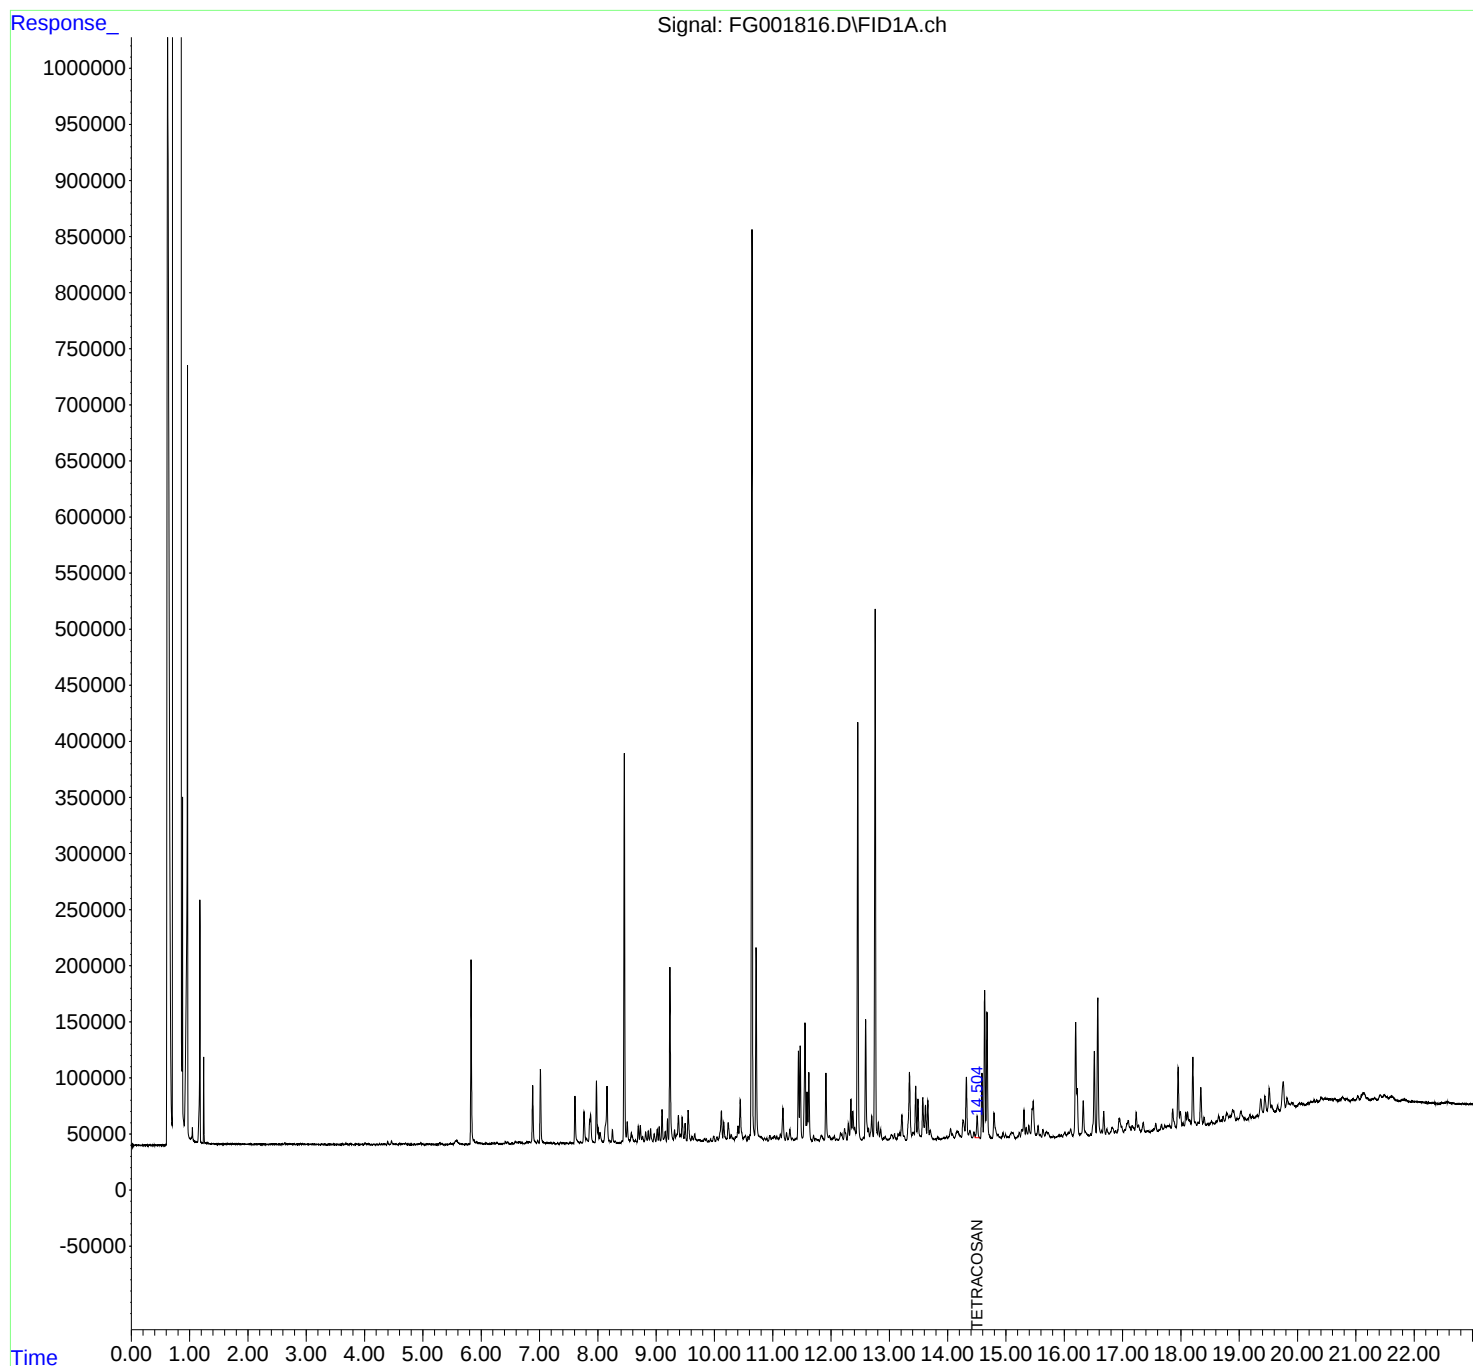

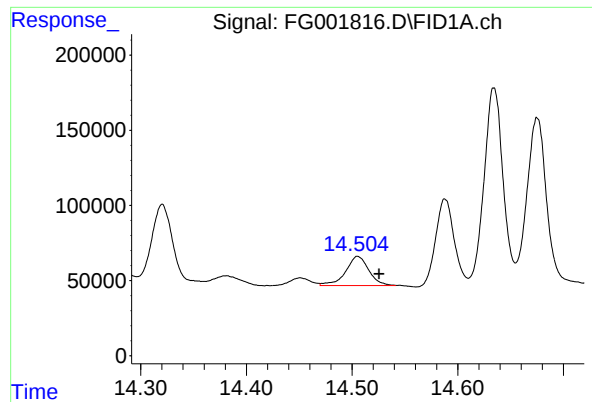

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.504 min
Delta R.T.: -0.021 min
Response: 295666
Conc: 2.54 ug/ml m

Instrument :
FID_G
ClientSampleId :
2018-NYSEG-CLARK-AREA-8

Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:00 AM