

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
 Data File : FG001827.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jul 2018 20:44
 Operator : AJ\SJ
 Sample : J4140-05MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Manual Integrations
 APPROVED

Sohil
 7/27/2018 10:03:02 AM

Integration File: autoint1.e
 Quant Time: Jul 27 04:20:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.505	3020696	25.964 ug/ml
Target Compounds			
2) N-DECANE	4.253	3582268	27.766 ug/ml
3) N-DODECANE	6.269	3645729	27.716 ug/ml
4) N-TETRADECANE	8.061	3750106	28.353 ug/ml
5) N-HEXADECANE	9.659	3724296	28.160 ug/ml
6) N-OCTADECANE	11.099	3694477	27.622 ug/ml
7) N-EICOSANE	12.408	3620031	27.119 ug/ml
8) N-DOCOSANE	13.605	3588853	26.970 ug/ml
10) N-TETRACOSANE	14.707	3695529	27.954 ug/mlm
11) N-HEXACOSANE	15.729	3492858	26.530 ug/ml
12) N-OCTACOSANE	16.679	3388624	25.920 ug/mlm

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072618\
Data File : FG001827.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2018 20:44
Operator : AJ\SJ
Sample : J4140-05MS
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:02 AM

Integration File: autoint1.e
Quant Time: Jul 27 04:20:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

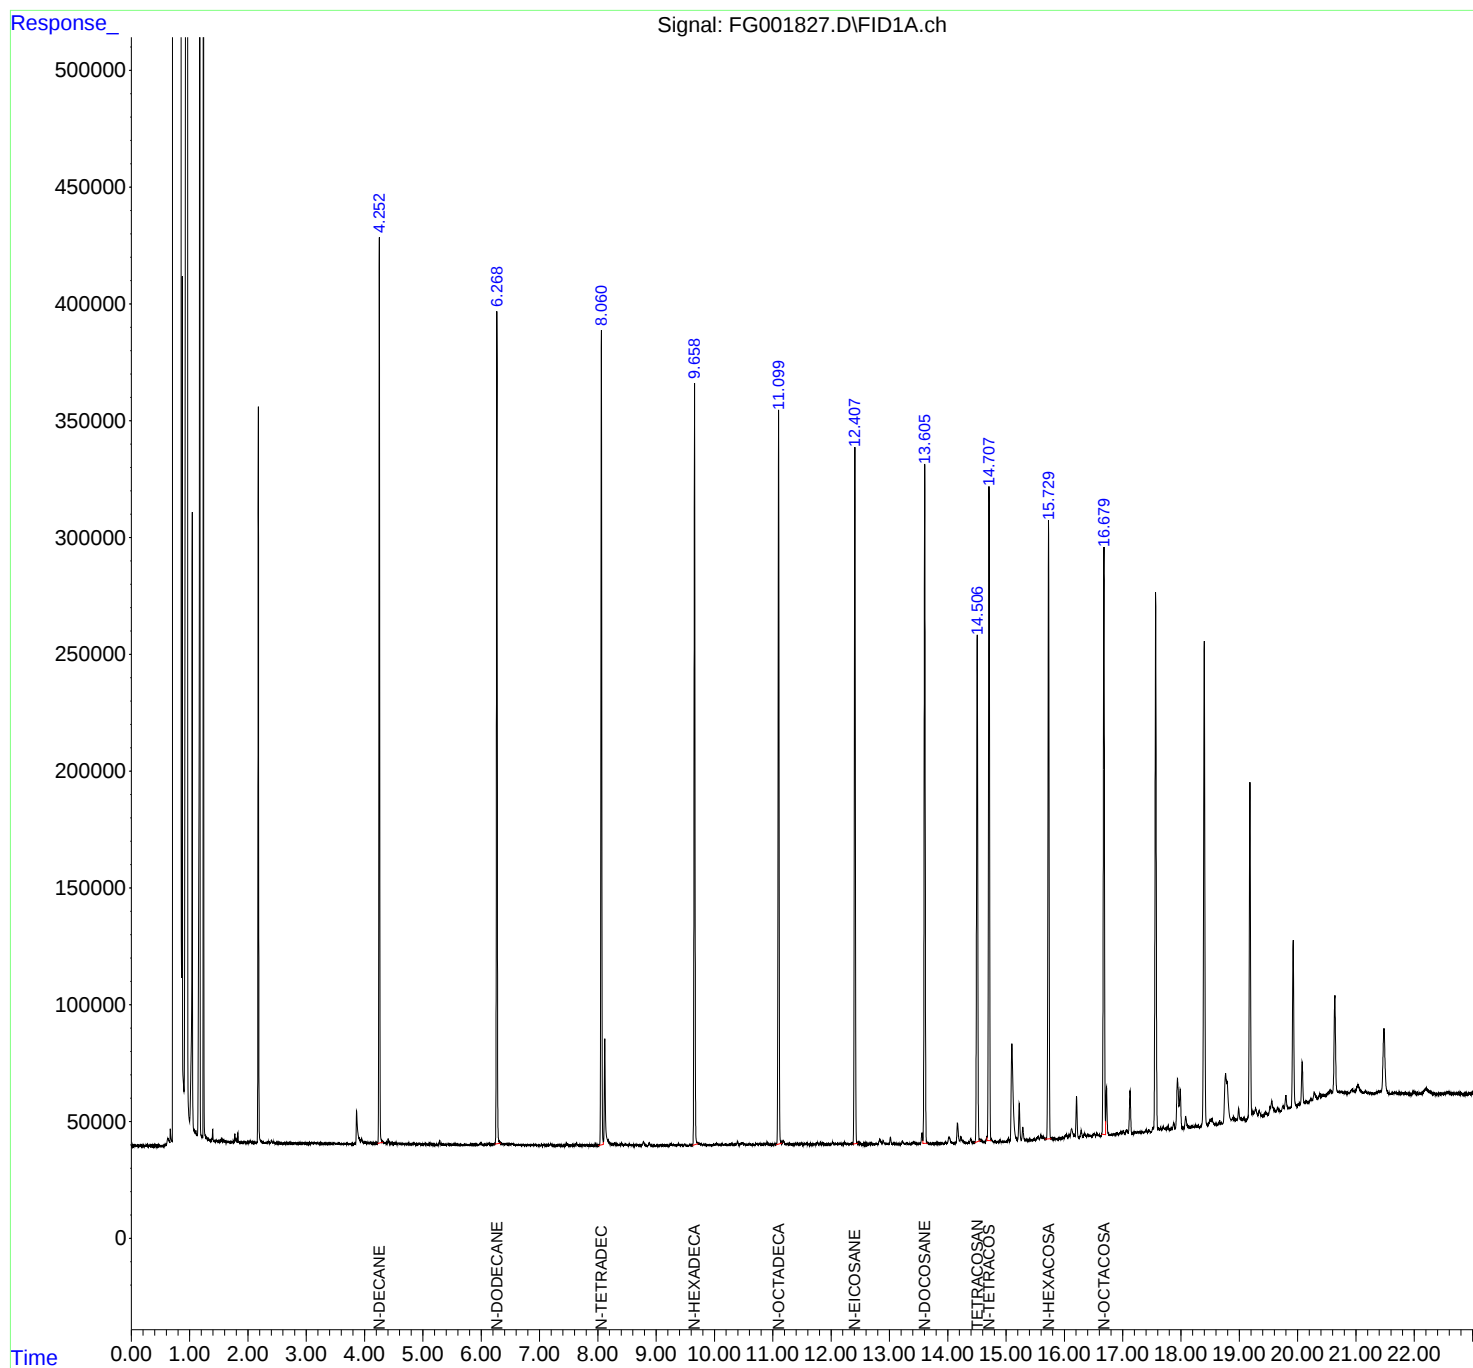

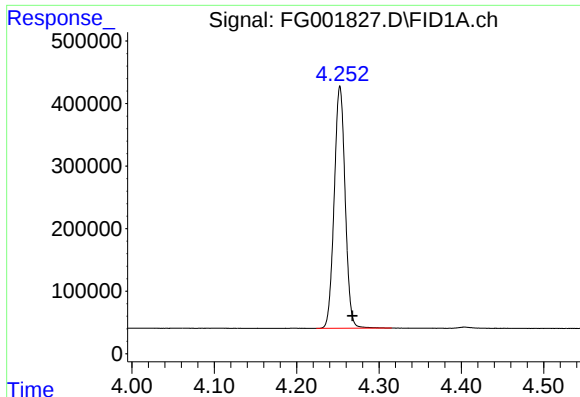


#2 N-DECANE

R.T.: 4.253 min
Delta R.T.: -0.015 min
Response: 3582268
Conc: 27.77 ug/ml

Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:02 AM

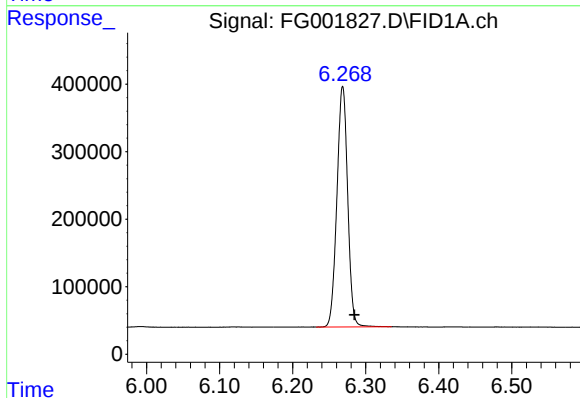


#3 N-DODECANE

R.T.: 6.269 min
Delta R.T.: -0.016 min
Response: 3645729
Conc: 27.72 ug/ml

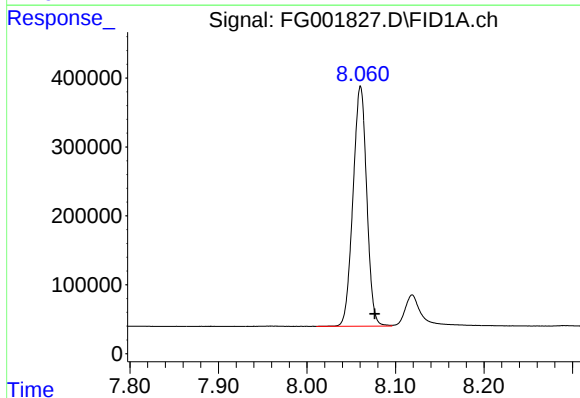


#4 N-TETRADECANE

R.T.: 8.061 min
Delta R.T.: -0.016 min
Response: 3750106
Conc: 28.35 ug/ml

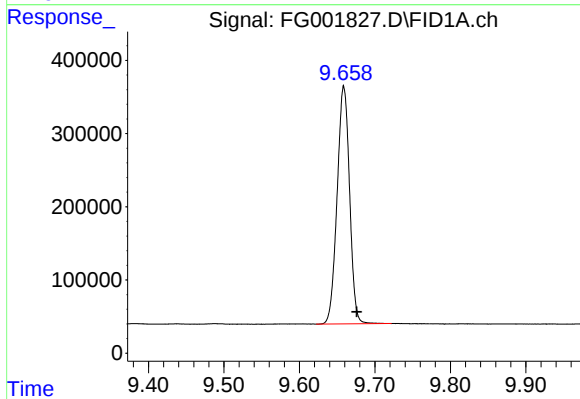

#5 N-HEXADECANE

R.T.: 9.659 min
Delta R.T.: -0.017 min
Response: 3724296
Conc: 28.16 ug/ml

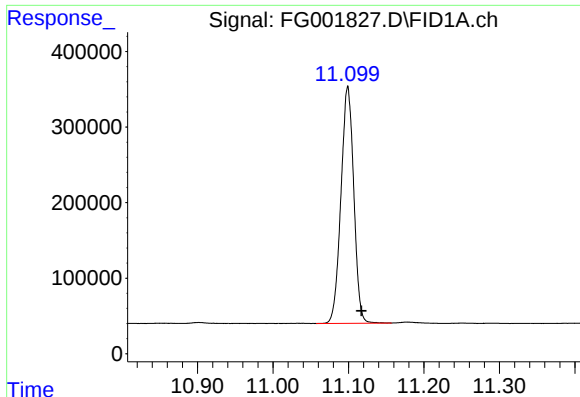


#6 N-OCTADECANE

R.T.: 11.099 min
Delta R.T.: -0.018 min
Response: 3694477
Conc: 27.62 ug/ml

Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:02 AM

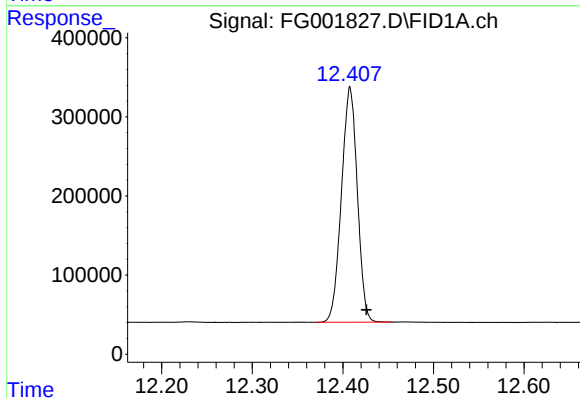


#7 N-EICOSANE

R.T.: 12.408 min
Delta R.T.: -0.018 min
Response: 3620031
Conc: 27.12 ug/ml

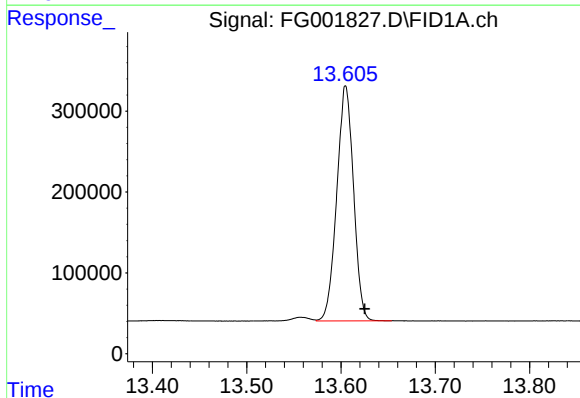


#8 N-DOCOSANE

R.T.: 13.605 min
Delta R.T.: -0.020 min
Response: 3588853
Conc: 26.97 ug/ml

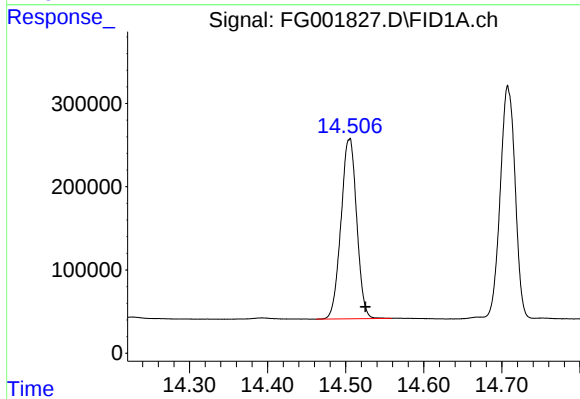

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.505 min
Delta R.T.: -0.021 min
Response: 3020696
Conc: 25.96 ug/ml

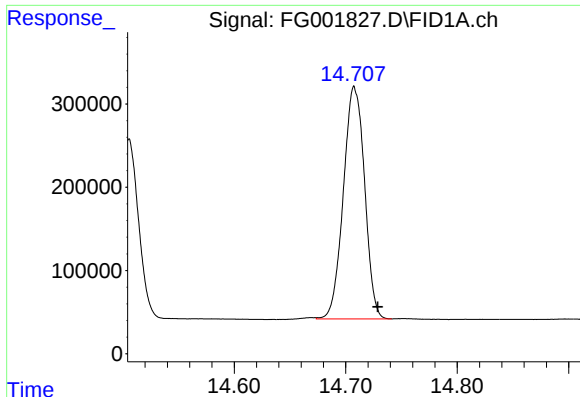


#10 N-TETRACOSANE

R.T.: 14.707 min
Delta R.T.: -0.022 min
Response: 3695529
Conc: 27.95 ug/ml m

Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

Sohil
7/27/2018 10:03:02 AM

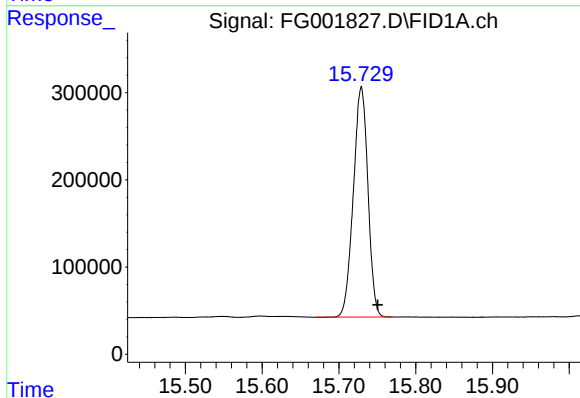

#11 N-HEXACOSANE

R.T.: 15.729 min
Delta R.T.: -0.021 min
Response: 3492858
Conc: 26.53 ug/ml

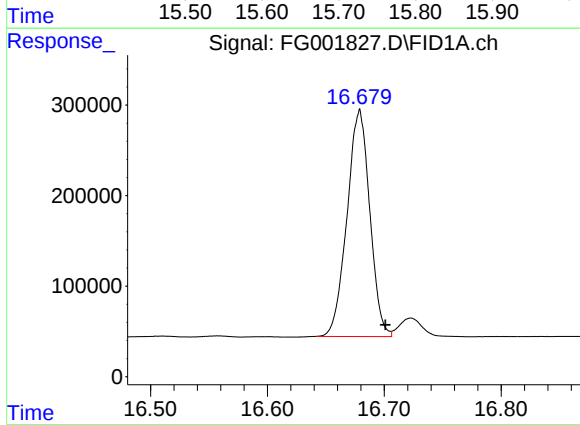

#12 N-OCTACOSANE

R.T.: 16.679 min
Delta R.T.: -0.022 min
Response: 3388624
Conc: 25.92 ug/ml m