

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072622\
Data File : FG010208.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2022 11:56
Operator : YP\AJ
Sample : PB146412BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 02:26:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.821	1933307	16.259 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.724	45475	0.384 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072622\
Data File : FG010208.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2022 11:56
Operator : YP\AJ
Sample : PB146412BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 02:26:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

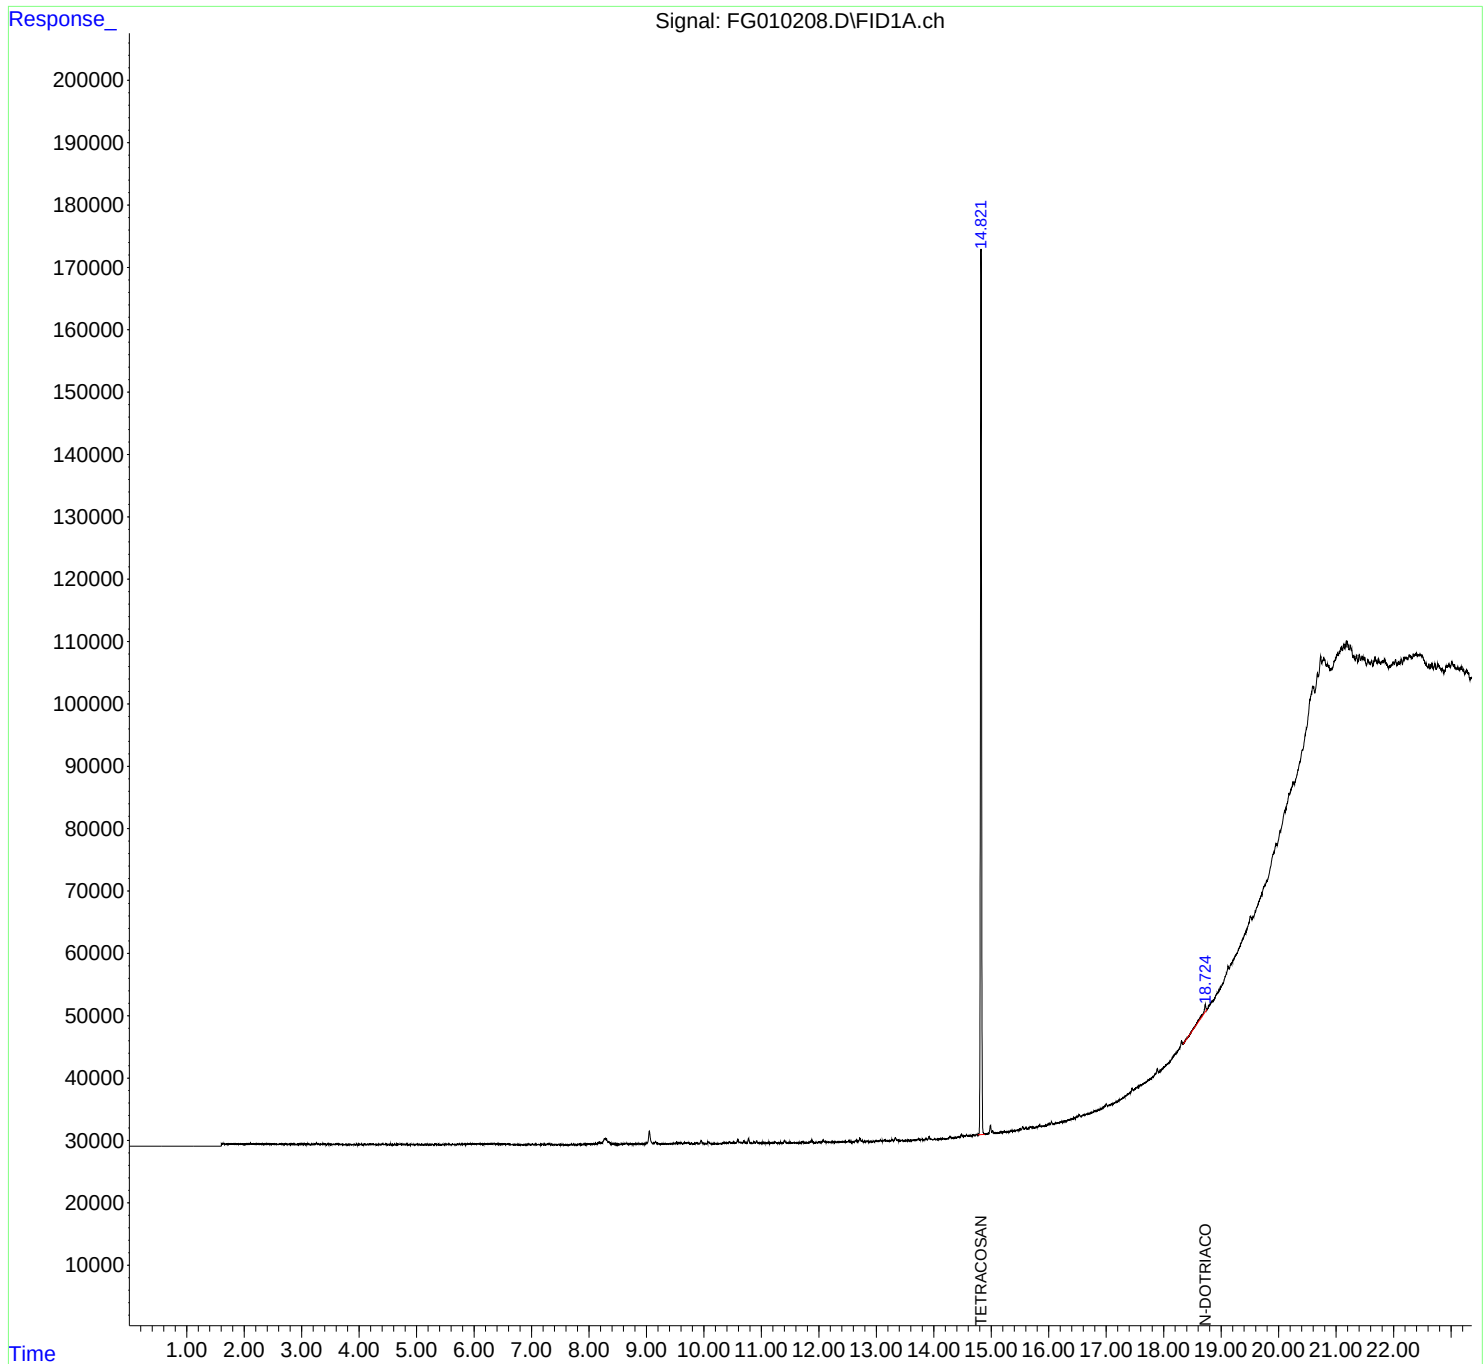


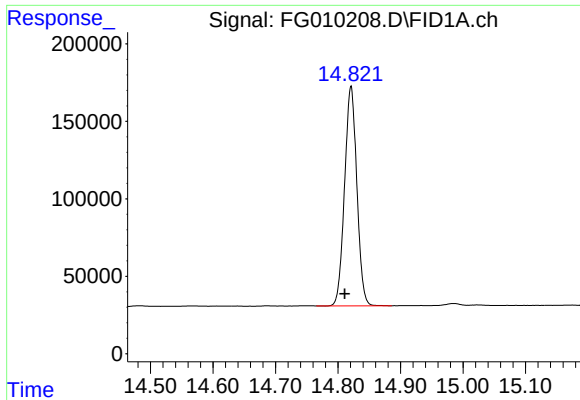

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.821 min
Delta R.T.: 0.010 min
Response: 1933307
Conc: 16.26 ug/ml

Instrument :
FID_G
ClientSampleId :

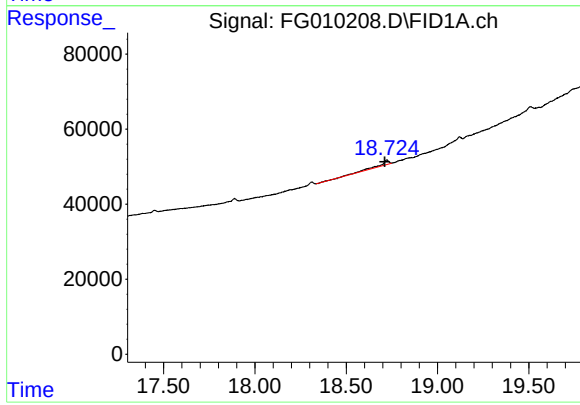

#14 N-DOTRIACONTANE

R.T.: 18.724 min
Delta R.T.: 0.012 min
Response: 45475
Conc: 0.38 ug/ml