

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072622\
Data File : FG010217.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2022 18:14
Operator : YP\AJ
Sample : PB146462BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 02:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.814	2297926	19.325 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.976	22154	0.167 ug/ml
13) N-TRIACONTANE	17.876	32350	0.257 ug/ml
18) N-TETRACONTANE	21.769	43791	0.559 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072622\
Data File : FG010217.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2022 18:14
Operator : YP\AJ
Sample : PB146462BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 02:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

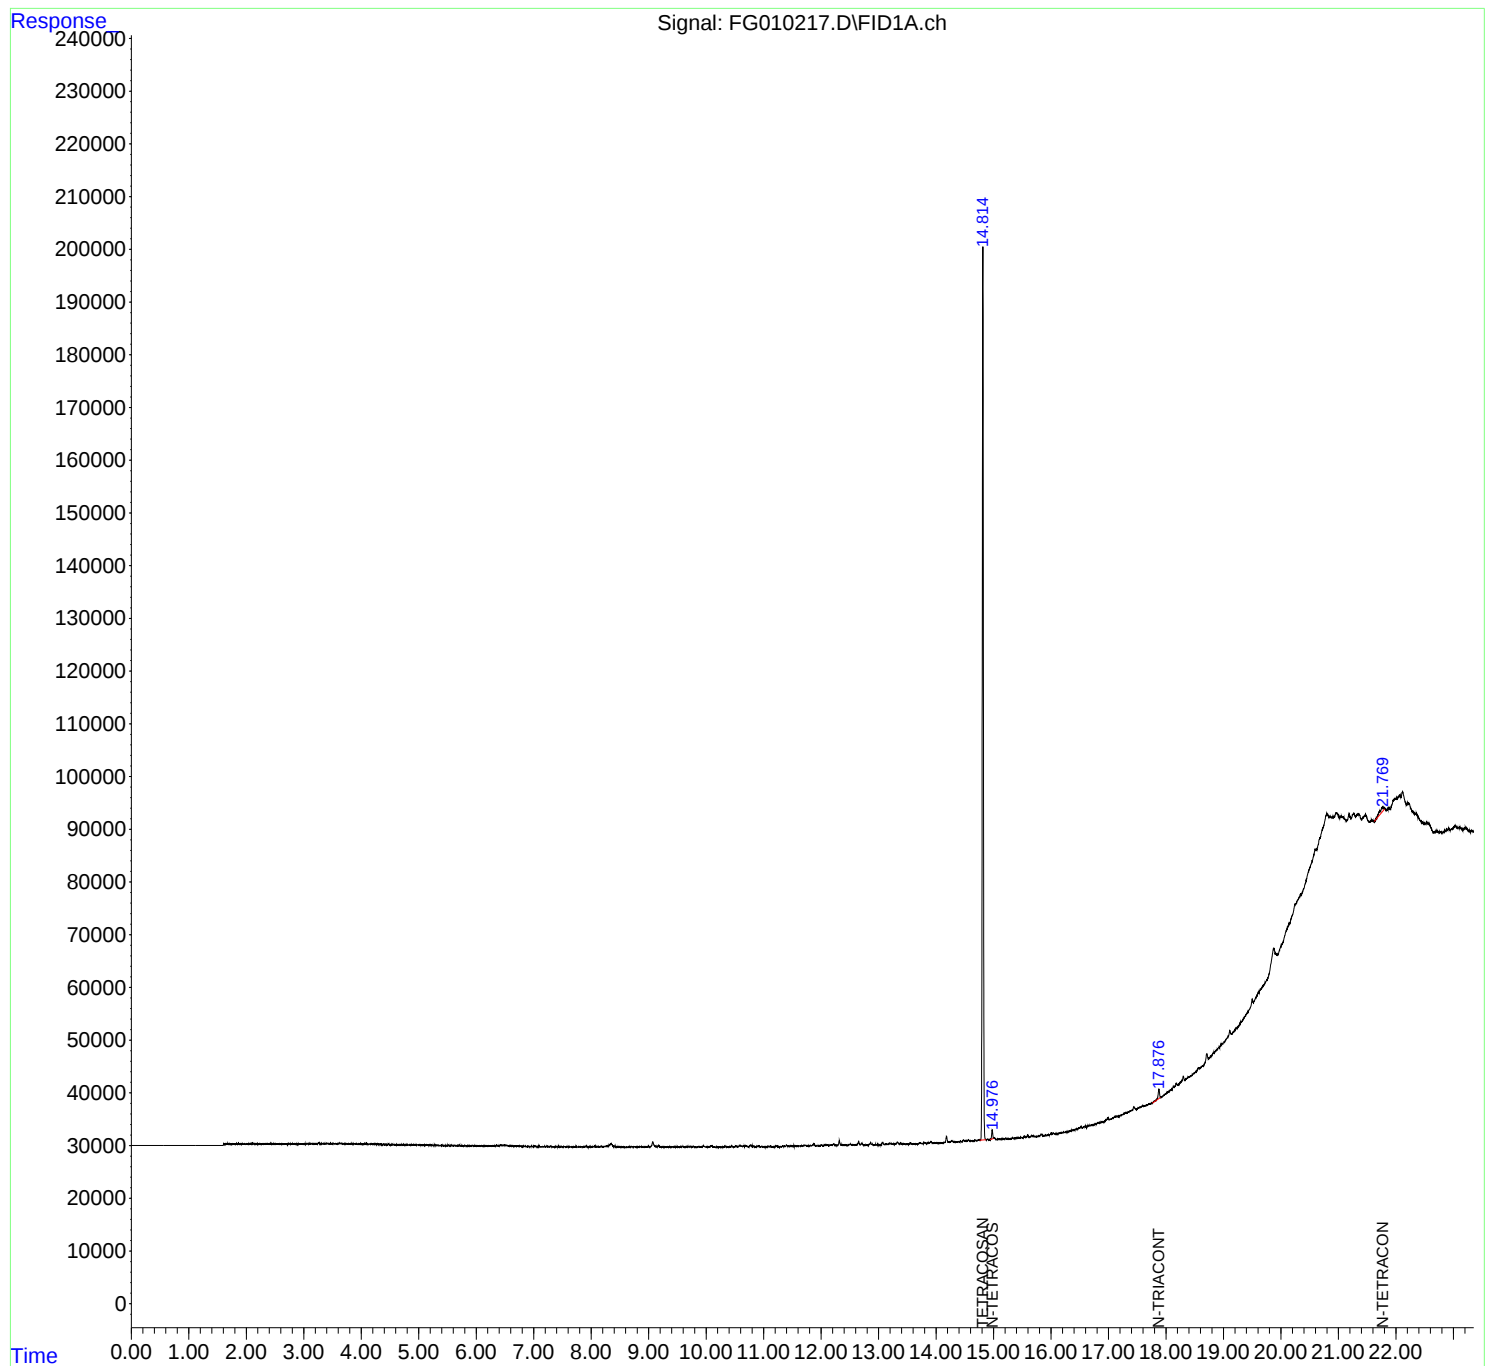


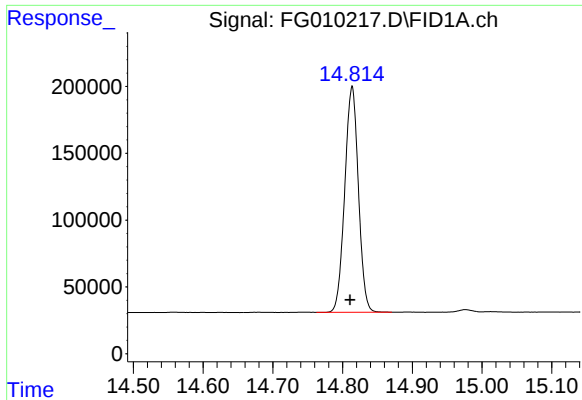

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.814 min
Delta R.T.: 0.003 min
Response: 2297926
Conc: 19.33 ug/ml

Instrument :
FID_G
ClientSampleId :

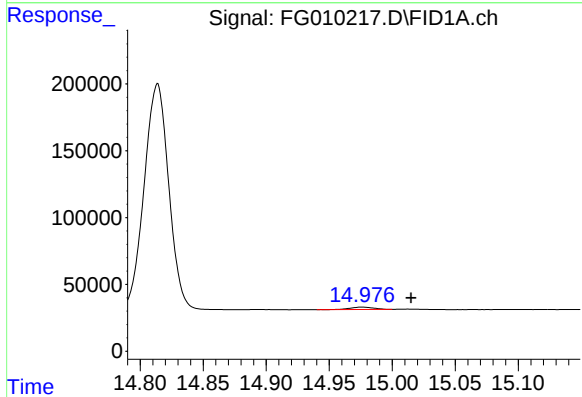


#10 N-TETRACOSANE

R.T.: 14.976 min
Delta R.T.: -0.039 min
Response: 22154
Conc: 0.17 ug/ml

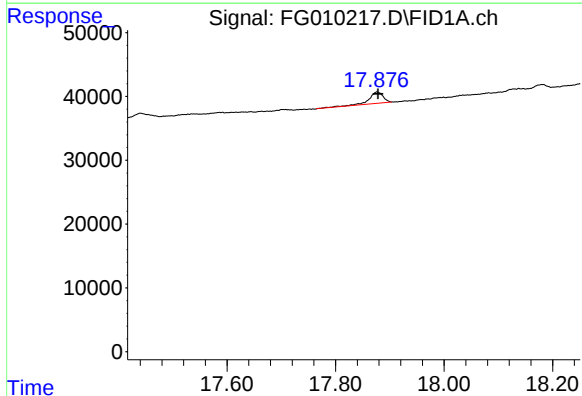

#13 N-TRIACONTANE

R.T.: 17.876 min
Delta R.T.: -0.002 min
Response: 32350
Conc: 0.26 ug/ml

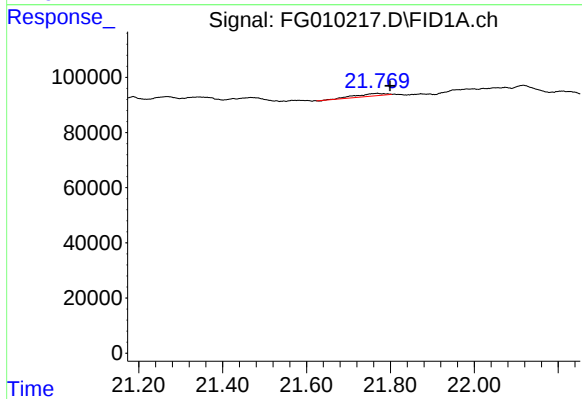

#18 N-TETRACONTANE

R.T.: 21.769 min
Delta R.T.: -0.030 min
Response: 43791
Conc: 0.56 ug/ml