

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072622\
Data File : FG010217.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2022 18:14
Operator : YP\AJ
Sample : PB146462BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB146462BL

Integration File: autoint1.e
Quant Time: Jul 27 02:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.814	2297926	19.325 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072622\
Data File : FG010217.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2022 18:14
Operator : YP\AJ
Sample : PB146462BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB146462BL

Integration File: autoint1.e
Quant Time: Jul 27 02:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

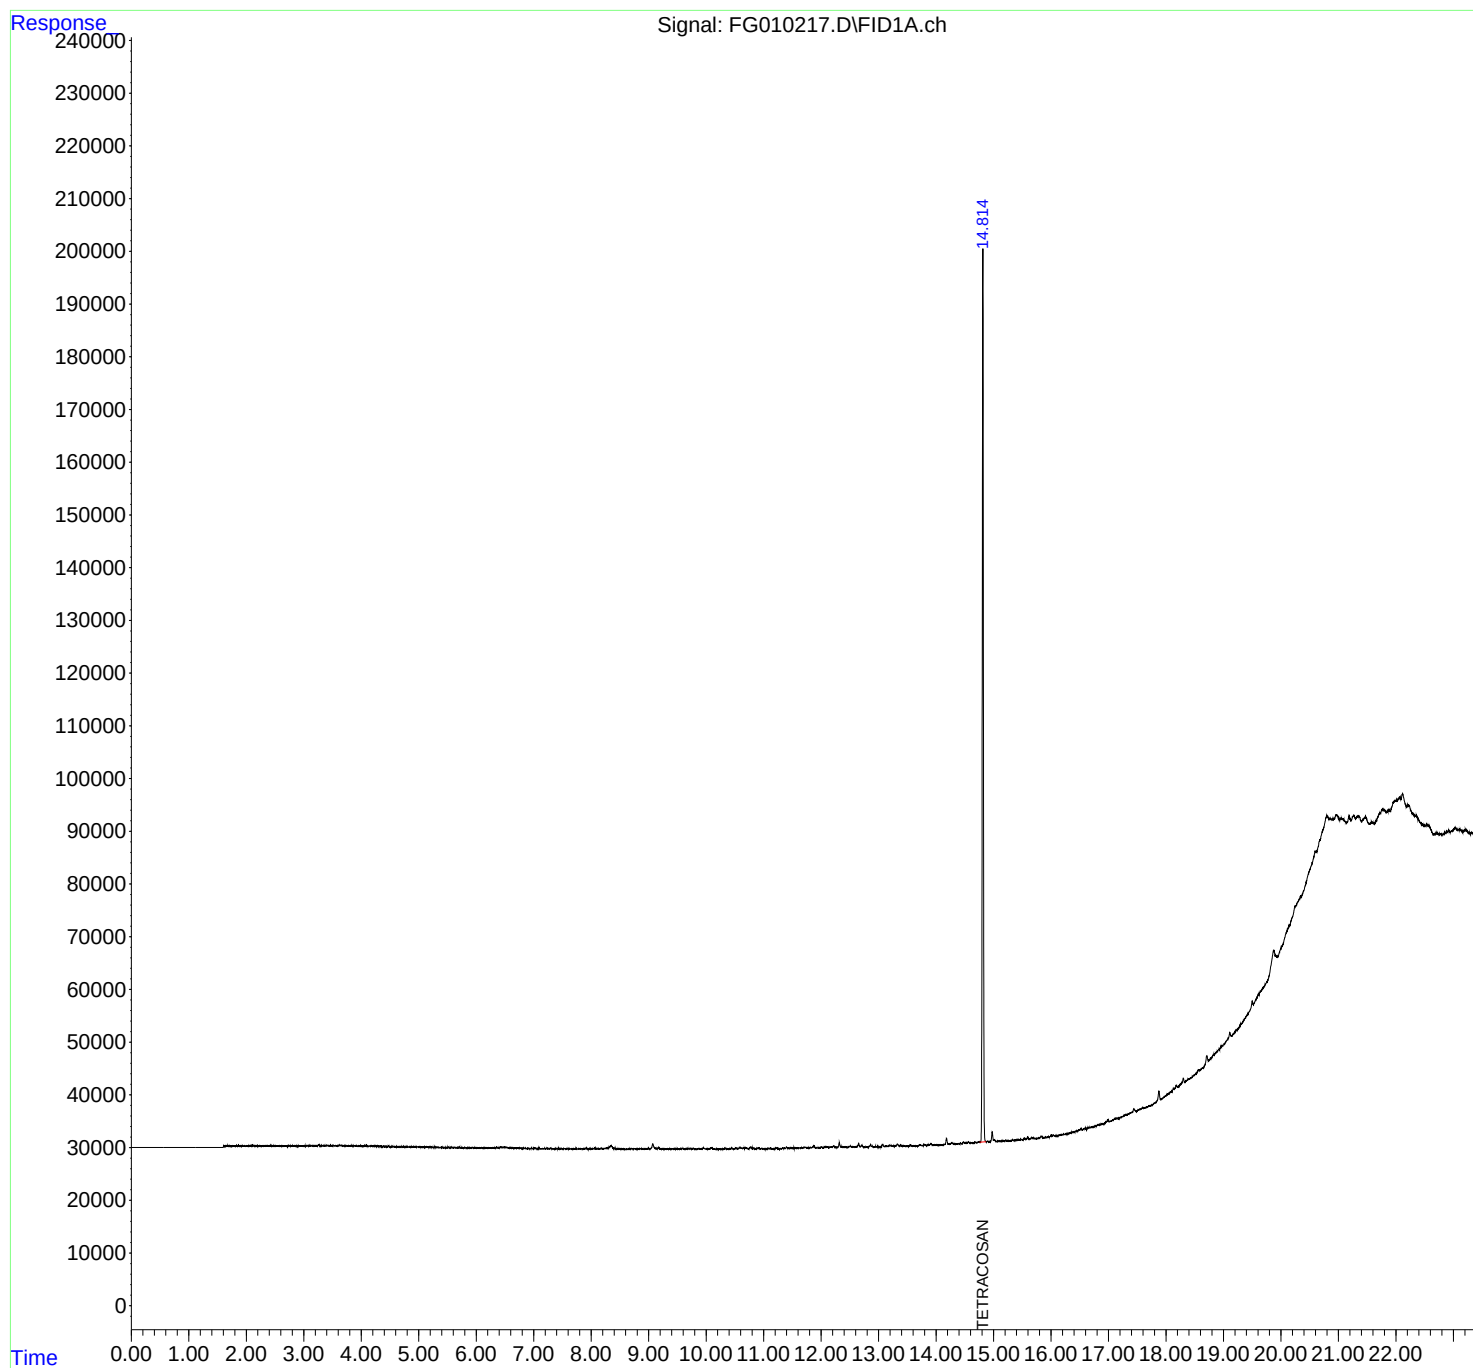

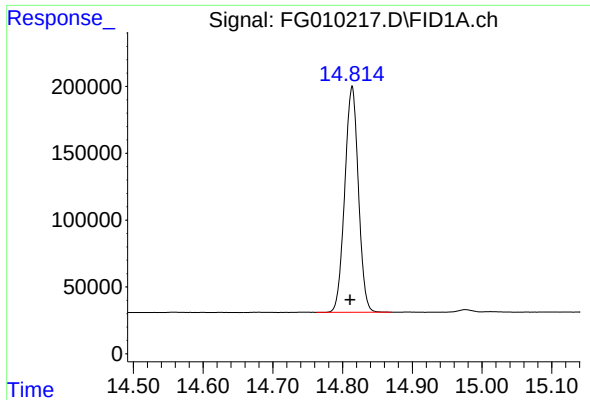

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.814 min
Delta R.T.: 0.003 min
Response: 2297926
Conc: 19.33 ug/ml

Instrument :
FID_G
ClientSampleId :
PB146462BL