

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072623\
 Data File : FG012560.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jul 2023 12:26
 Operator : YP\AJ
 Sample : PB154425BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 27 02:34:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
 Quant Title :
 QLast Update : Thu Jul 06 13:57:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.979	1983463	18.560 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.163	176117	1.331 ug/ml
15) N-TETRATRIACONTANE	19.663	33663	0.342 ug/ml
16) N-HEXATRIACONTANE	20.444	98427	1.064 ug/ml
18) N-TETRACONTANE	22.057	134801	1.518 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072623\
Data File : FG012560.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2023 12:26
Operator : YP\AJ
Sample : PB154425BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 27 02:34:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

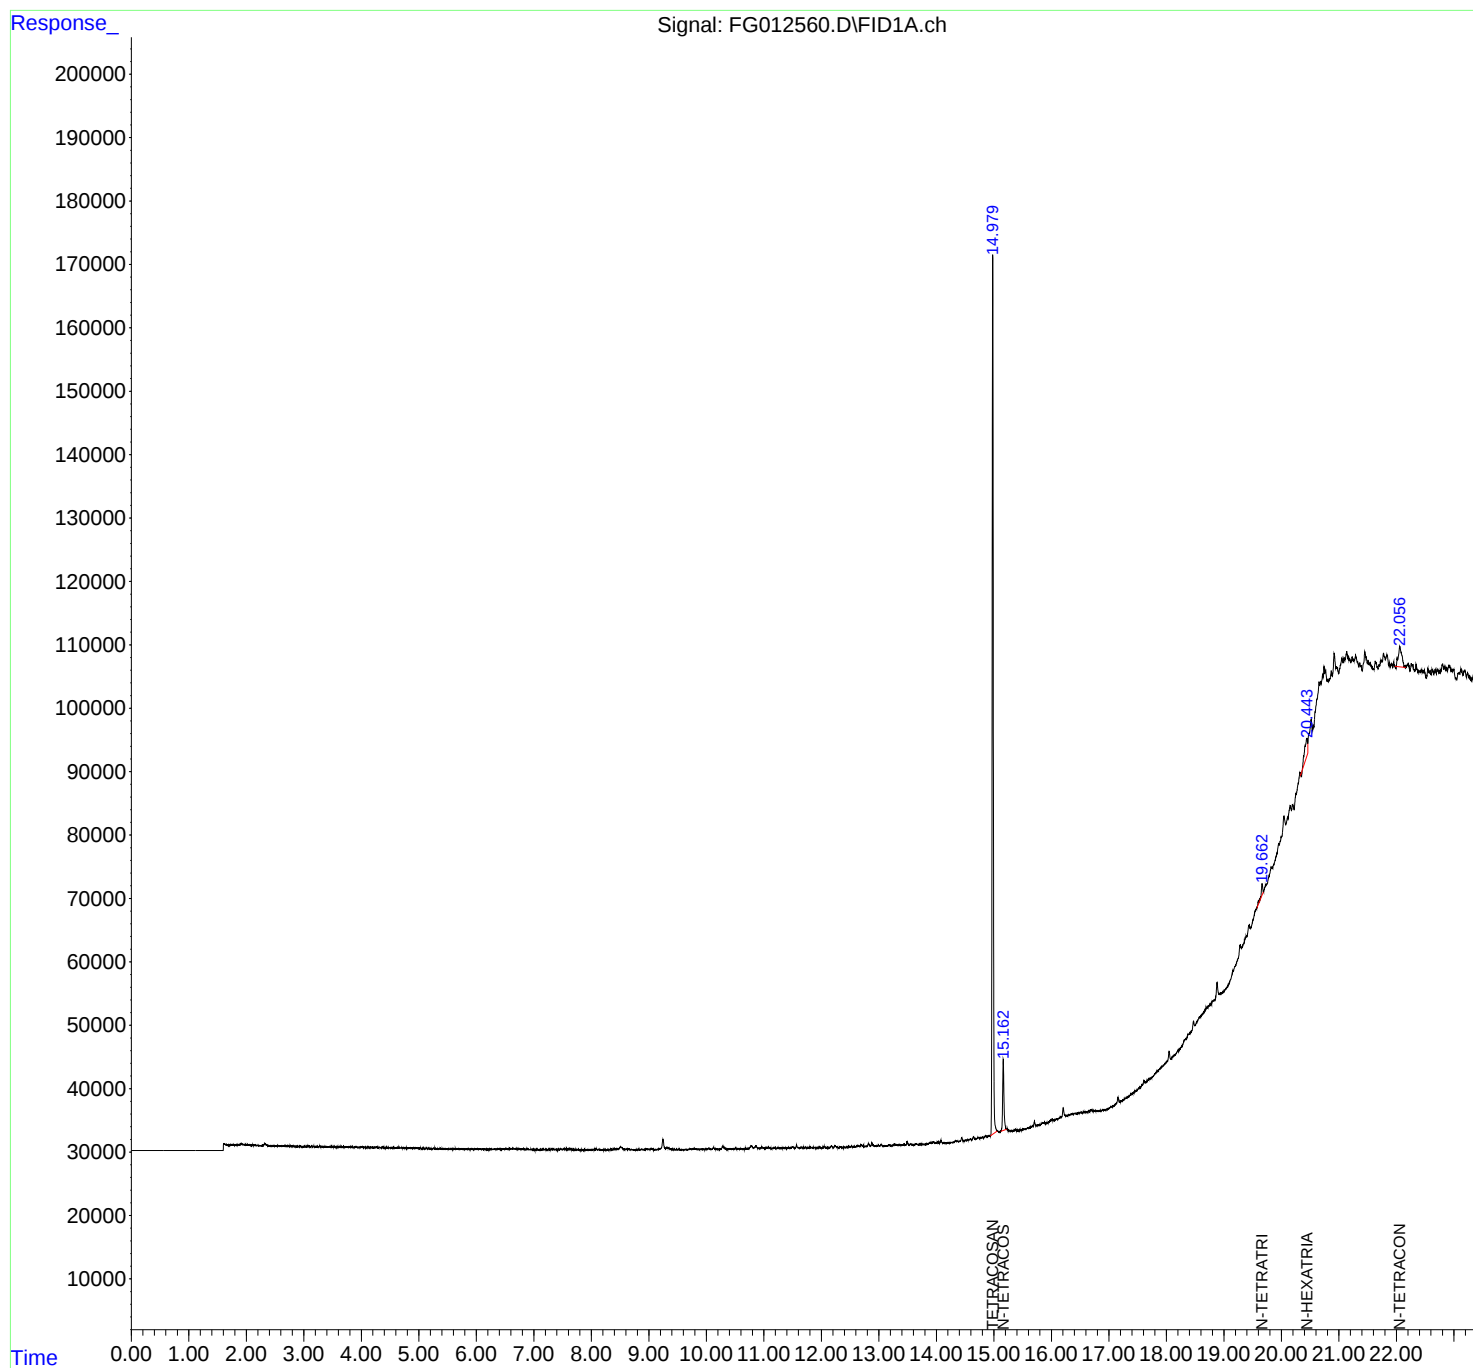


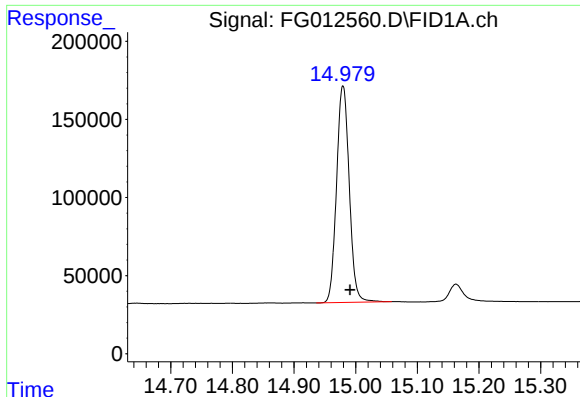

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.979 min
Delta R.T.: -0.012 min
Response: 1983463
Conc: 18.56 ug/ml

Instrument :
FID_G
ClientSampleId :

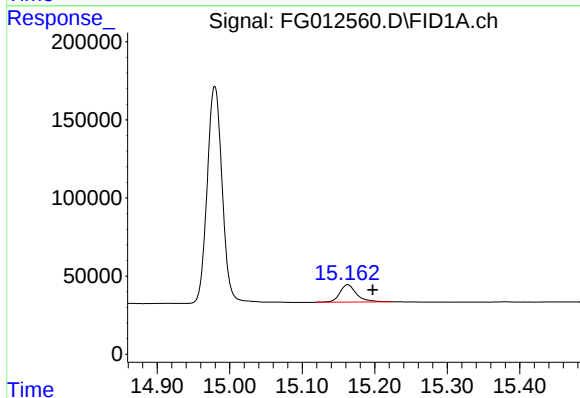


#10 N-TETRACOSANE

R.T.: 15.163 min
Delta R.T.: -0.034 min
Response: 176117
Conc: 1.33 ug/ml

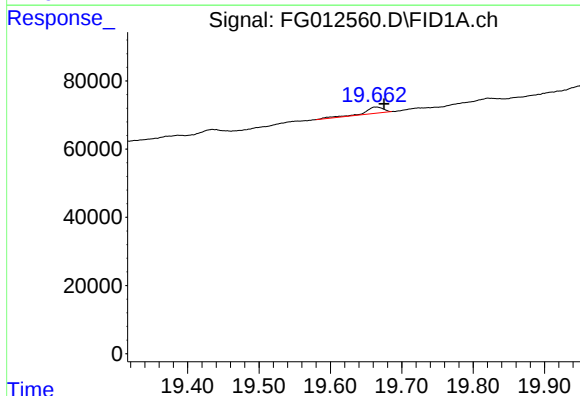


#15 N-TETRATRIACONTANE

R.T.: 19.663 min
Delta R.T.: -0.012 min
Response: 33663
Conc: 0.34 ug/ml

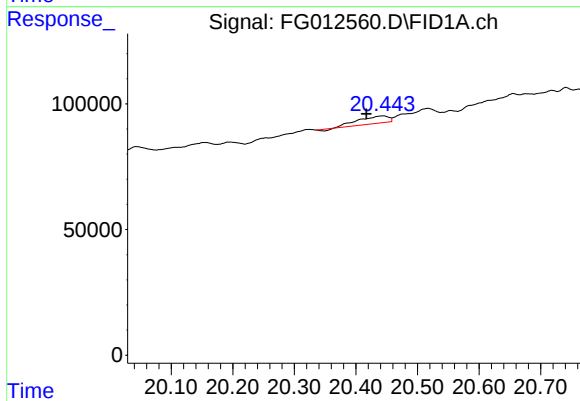

#16 N-HEXATRIACONTANE

R.T.: 20.444 min
Delta R.T.: 0.027 min
Response: 98427
Conc: 1.06 ug/ml

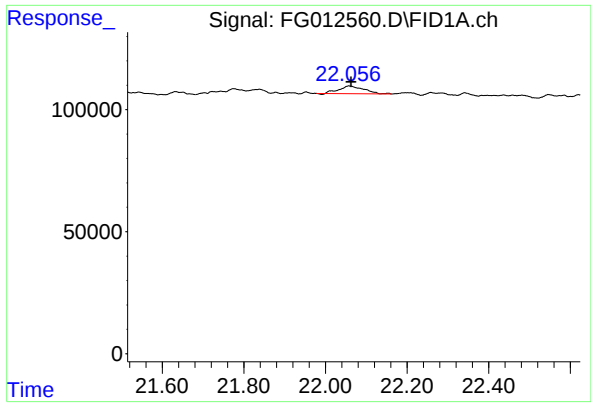

#18 N-TETRACONTANE

R.T.: 22.057 min
Delta R.T.: -0.006 min
Response: 134801
Conc: 1.52 ug/ml

Instrument :
FID_G
ClientSampleId :