

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072623\
 Data File : FG012564.D
 Signal(s) : FID1A.ch
 Acq On : 26 Jul 2023 14:24
 Operator : YP\AJ
 Sample : 03742-01MSD
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 WC-27MSD

Integration File: Sample.e
 Quant Time: Jul 27 02:36:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
 Quant Title :
 QLast Update : Thu Jul 06 13:57:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.977	1261922	11.809 ug/ml
Target Compounds			
2) N-DECANE	4.515	2251336	18.470 ug/ml
3) N-DODECANE	6.685	2290260	18.695 ug/ml
4) N-TETRADECANE	8.514	2270261	19.104 ug/ml
5) N-HEXADECANE	10.123	2284638	18.220 ug/ml
6) N-OCTADECANE	11.568	2318098	18.045 ug/ml
7) N-EICOSANE	12.878	2267545	17.952 ug/ml
8) N-DOCOSANE	14.078	2206557	17.959 ug/ml
10) N-TETRACOSANE	15.182	2346669	17.738 ug/ml
11) N-HEXACOSANE	16.205	2108831	18.021 ug/ml
12) N-OCTACOSANE	17.156	2154515	18.870 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072623\
Data File : FG012564.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2023 14:24
Operator : YP\AJ
Sample : 03742-01MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC-27MSD

Integration File: Sample.e
Quant Time: Jul 27 02:36:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070623.M
Quant Title :
QLast Update : Thu Jul 06 13:57:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

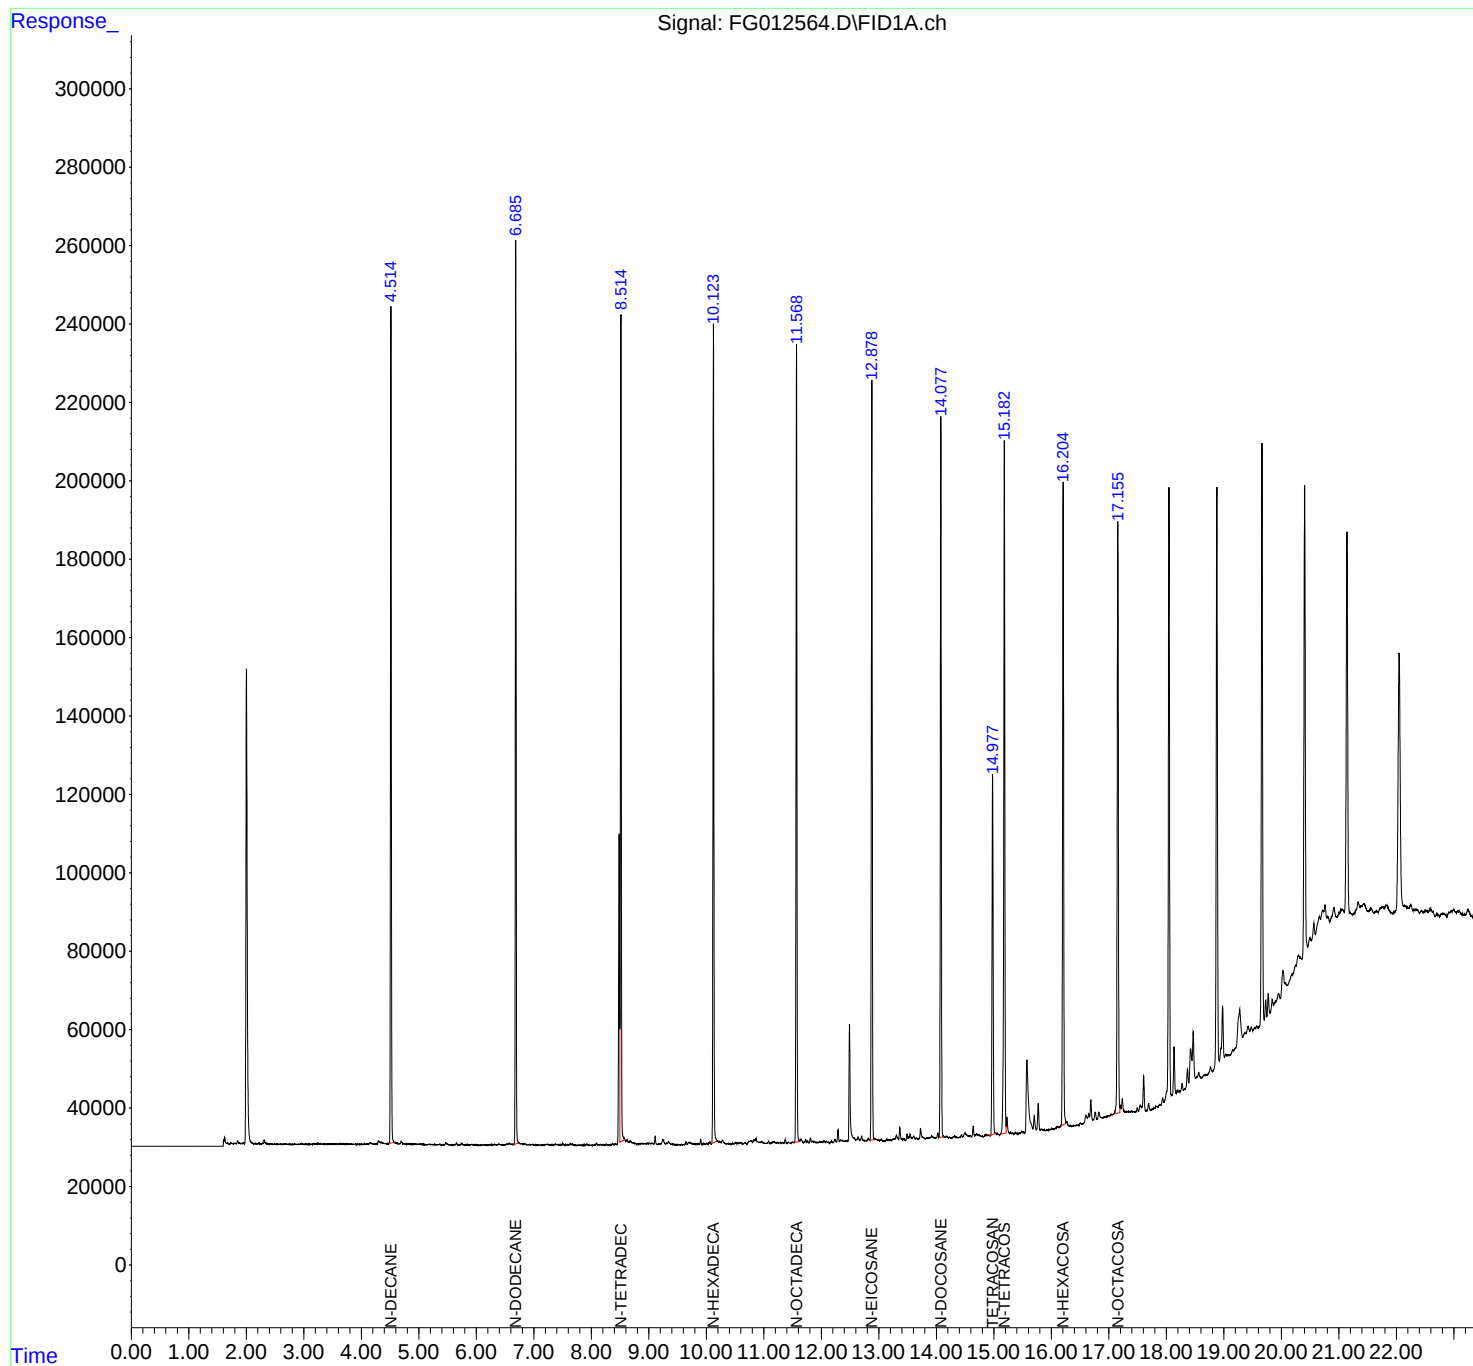


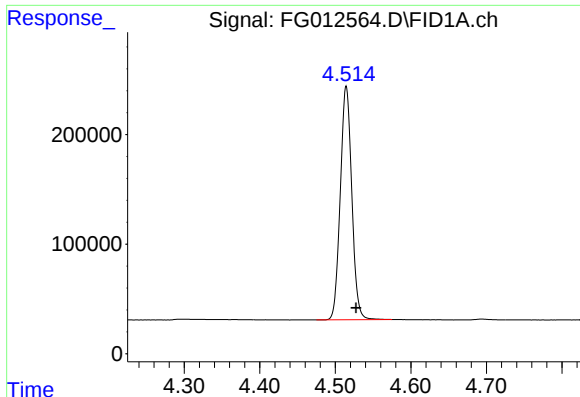

#2 N-DECANE


R.T.: 4.515 min
Delta R.T.: -0.013 min
Response: 2251336
Conc: 18.47 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-27MSD

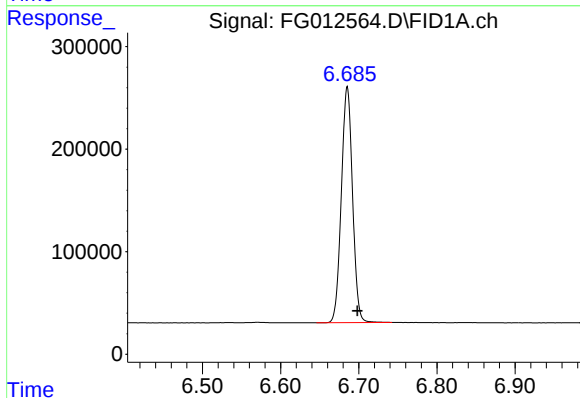


#3 N-DODECANE

R.T.: 6.685 min
Delta R.T.: -0.013 min
Response: 2290260
Conc: 18.69 ug/ml

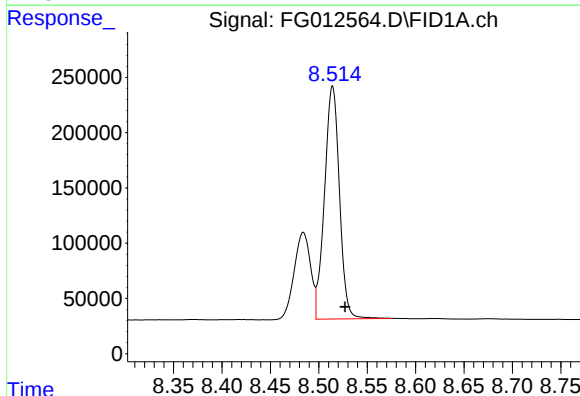


#4 N-TETRADECANE

R.T.: 8.514 min
Delta R.T.: -0.013 min
Response: 2270261
Conc: 19.10 ug/ml

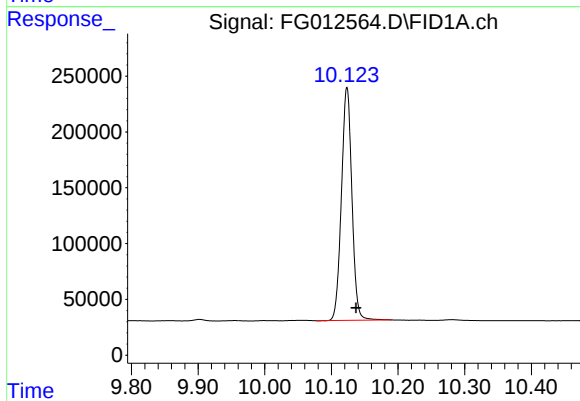

#5 N-HEXADECANE


R.T.: 10.123 min
Delta R.T.: -0.013 min
Response: 2284638
Conc: 18.22 ug/ml

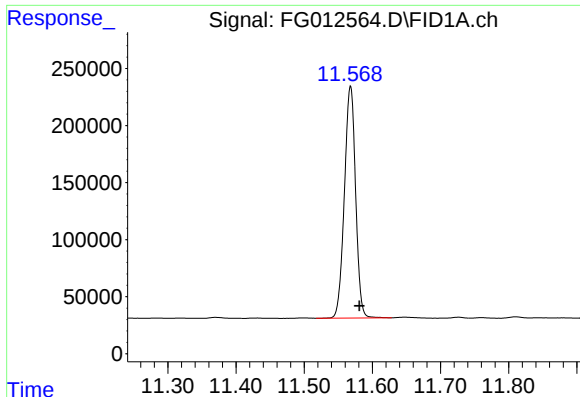

#6 N-OCTADECANE


R.T.: 11.568 min
Delta R.T.: -0.013 min
Response: 2318098
Conc: 18.05 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-27MSD

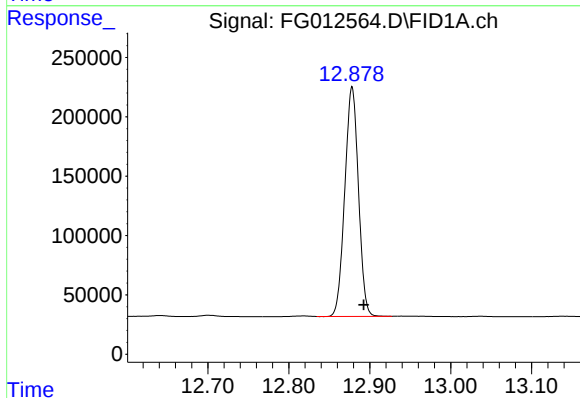


#7 N-EICOSANE

R.T.: 12.878 min
Delta R.T.: -0.014 min
Response: 2267545
Conc: 17.95 ug/ml

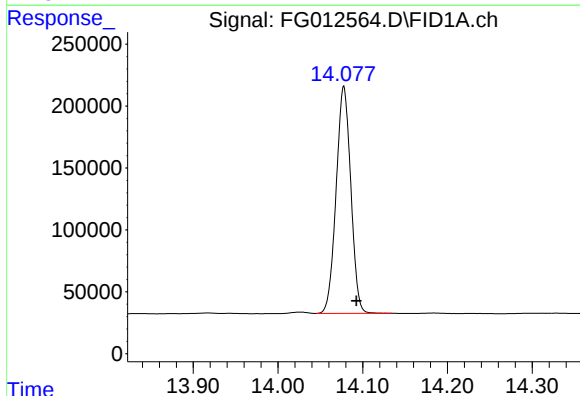


#8 N-DOCOSANE

R.T.: 14.078 min
Delta R.T.: -0.015 min
Response: 2206557
Conc: 17.96 ug/ml

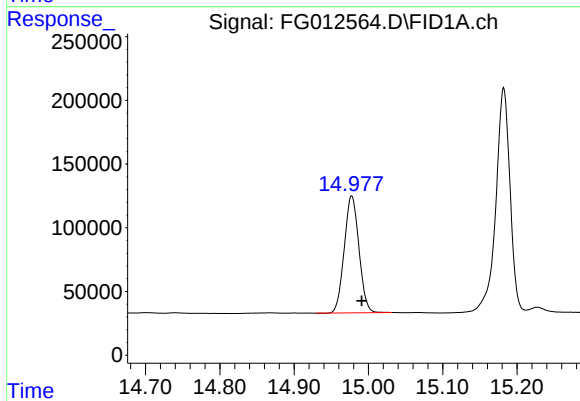

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.977 min
Delta R.T.: -0.014 min
Response: 1261922
Conc: 11.81 ug/ml

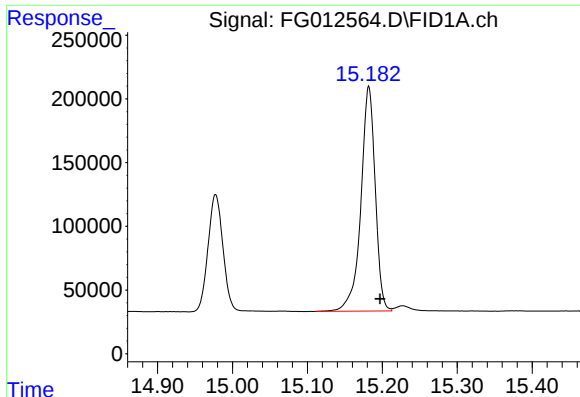

#10 N-TETRACOSANE


R.T.: 15.182 min
Delta R.T.: -0.015 min
Response: 2346669
Conc: 17.74 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-27MSD

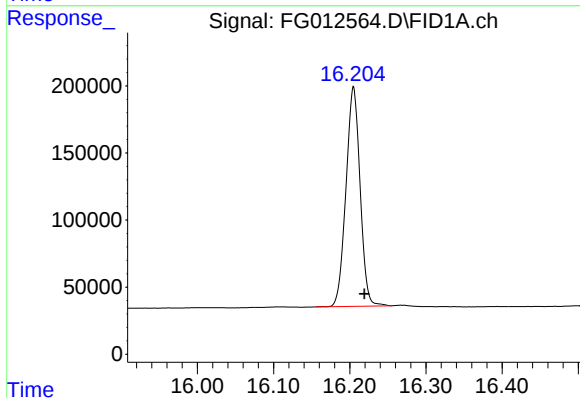

#11 N-HEXACOSANE

R.T.: 16.205 min
Delta R.T.: -0.014 min
Response: 2108831
Conc: 18.02 ug/ml

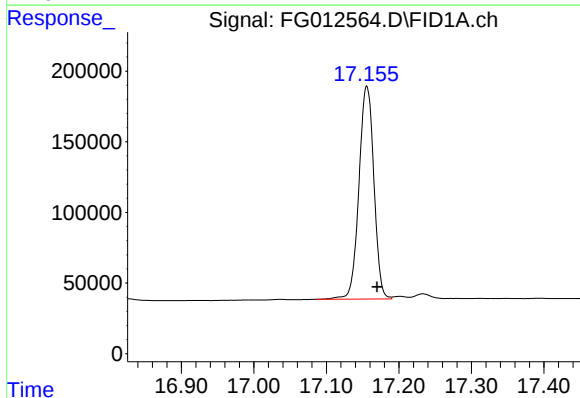

#12 N-OCTACOSANE

R.T.: 17.156 min
Delta R.T.: -0.014 min
Response: 2154515
Conc: 18.87 ug/ml