

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072624\
Data File : FG013965.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2024 12:14
Operator : YP\AJ
Sample : P3341-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-05-072324

Integration File: autoint1.e
Quant Time: Jul 27 02:54:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.955	1996826	16.507 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072624\
Data File : FG013965.D
Signal(s) : FID1A.ch
Acq On : 26 Jul 2024 12:14
Operator : YP\AJ
Sample : P3341-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-05-072324

Integration File: autoint1.e
Quant Time: Jul 27 02:54:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

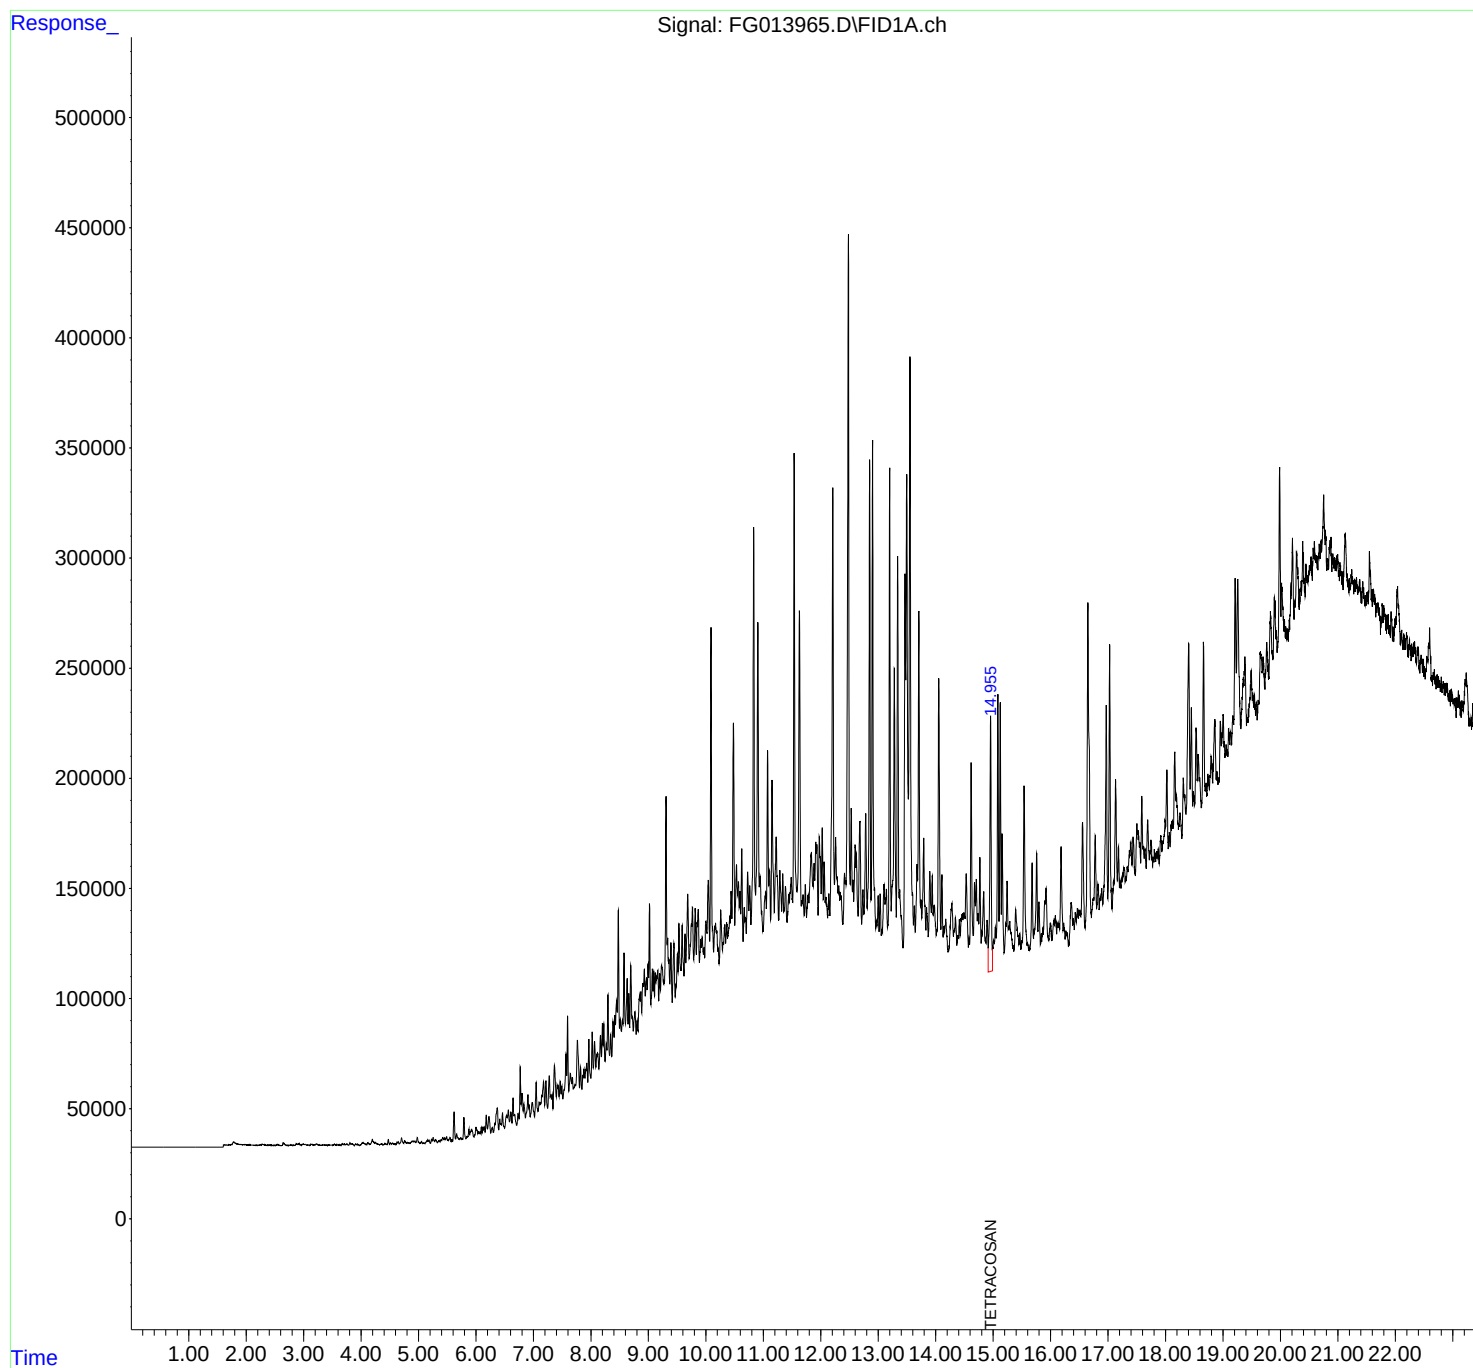

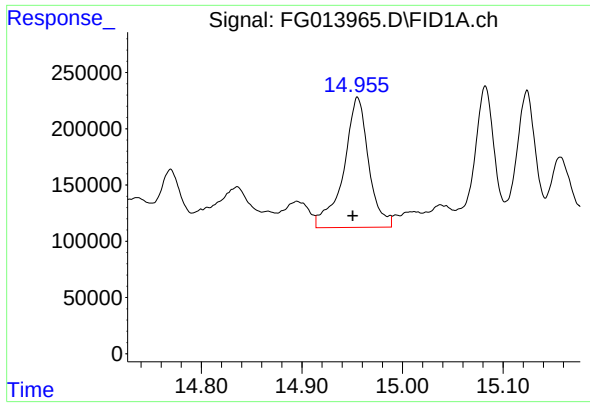

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.955 min
Delta R.T.: 0.005 min
Response: 1996826
Conc: 16.51 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-05-072324