

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG073124\
Data File : FG013997.D
Signal(s) : FID1A.ch
Acq On : 31 Jul 2024 16:18
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 03:03:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.643	2373488	17.988 ug/ml
12)	N-OCTACOSANE	17.131	2330397	18.373 ug/ml
13)	N-TRIACONTANE	18.019	71502	0.568 ug/ml
14)	N-DOTRIACONTANE	18.854	115641	0.948 ug/ml
15)	N-TETRATRIACONTANE	19.639	93719	0.931 ug/ml
16)	N-HEXATRIACONTANE	20.384	148547	1.778 ug/ml
17)	N-OCTATRIACONTANE	21.115	114536	1.536 ug/ml
18)	N-TETRACONTANE	22.016	135315	1.953 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG073124\
Data File : FG013997.D
Signal(s) : FID1A.ch
Acq On : 31 Jul 2024 16:18
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 01 03:03:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

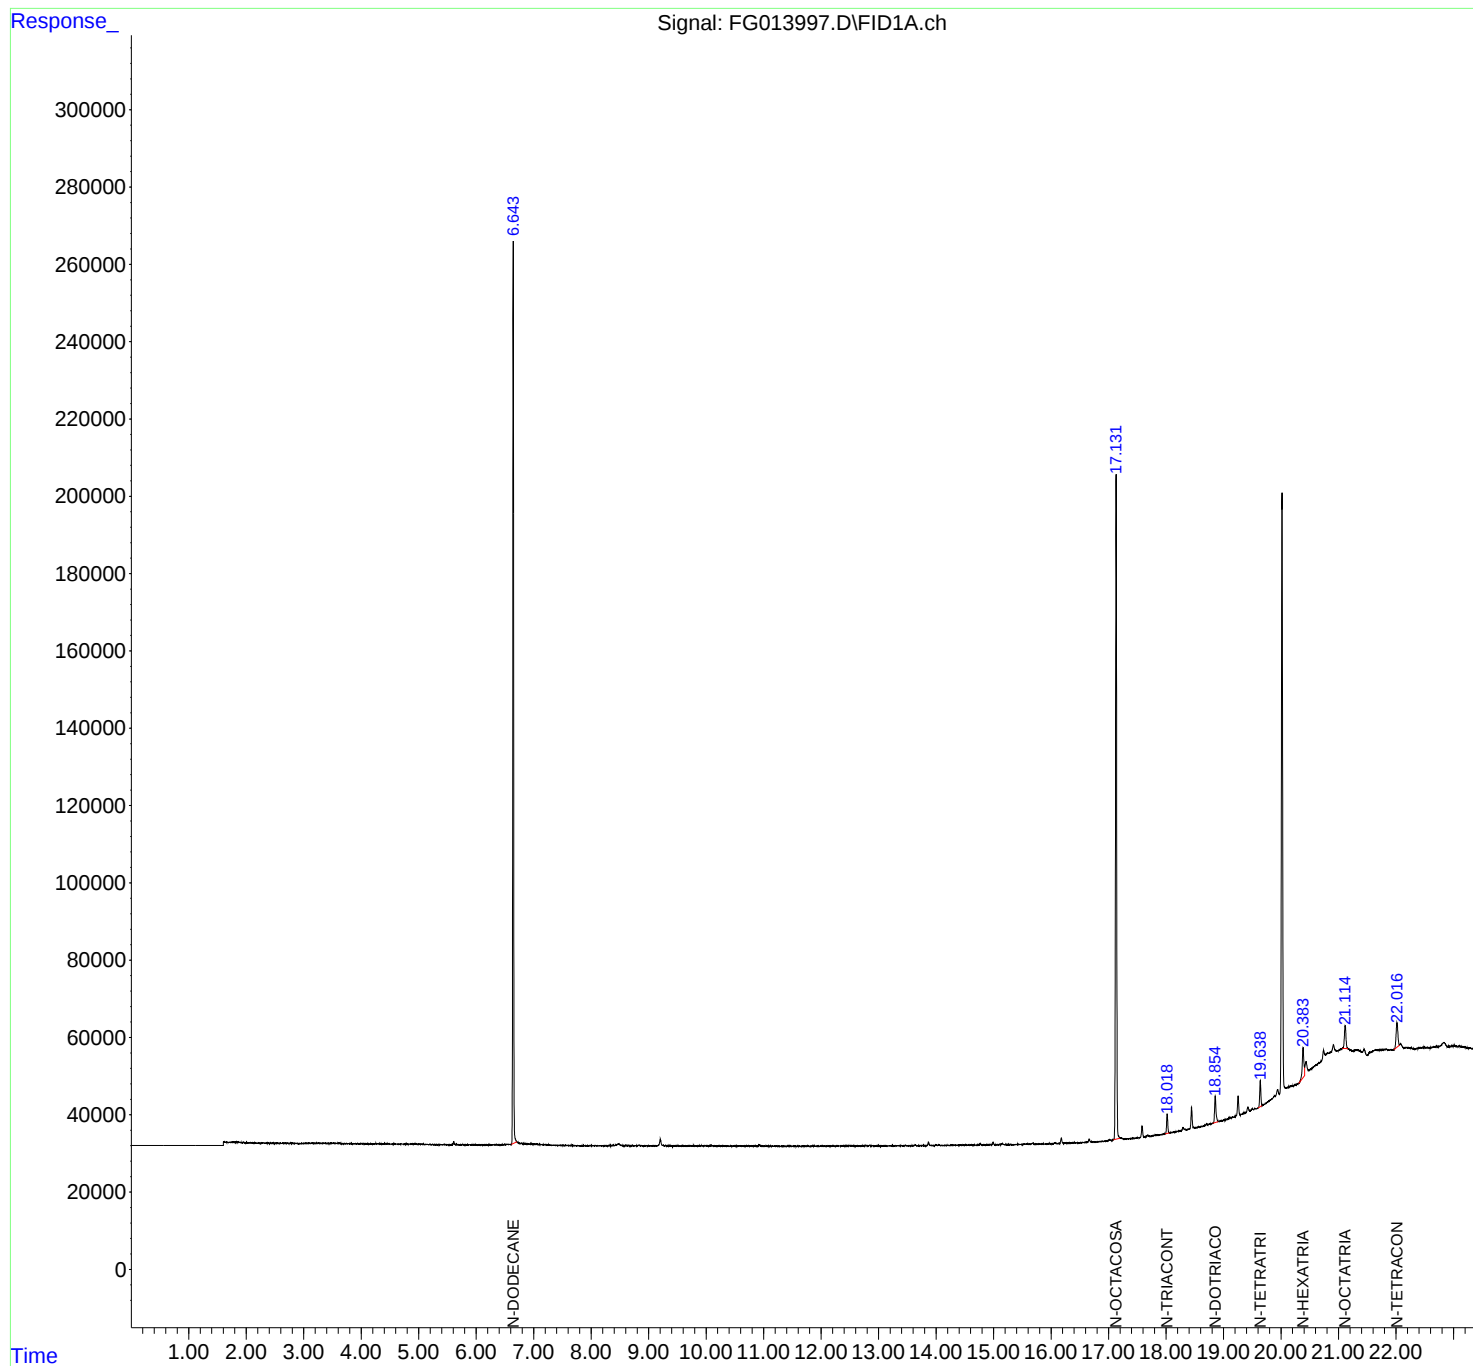


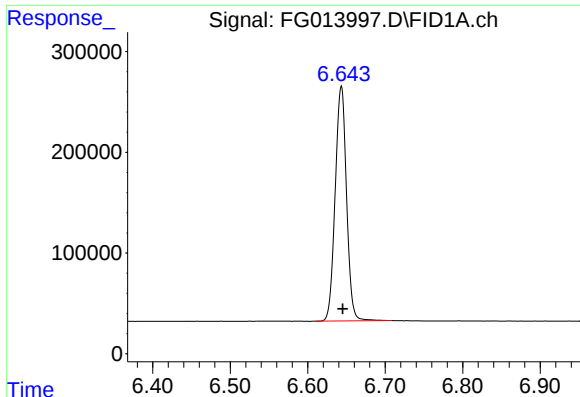

#3 N-DODECANE


R.T.: 6.643 min
Delta R.T.: -0.002 min
Response: 2373488
Conc: 17.99 ug/ml

Instrument :
FID_G
ClientSampleId :

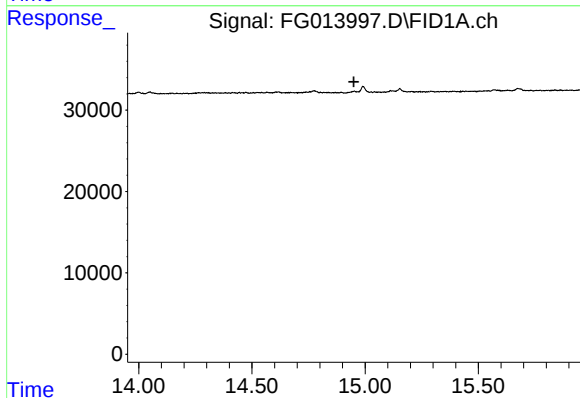


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.950 min
Response: 0
Conc: N.D.

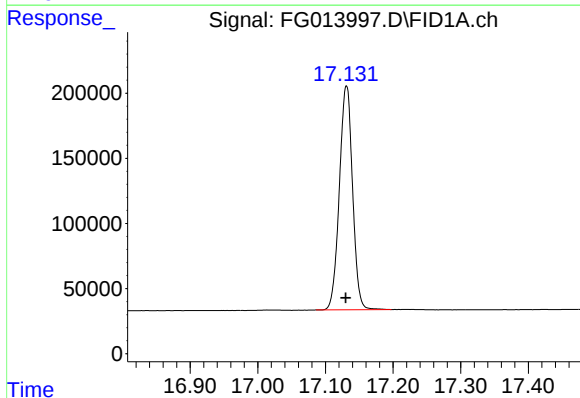


#12 N-OCTACOSANE

R.T.: 17.131 min
Delta R.T.: 0.000 min
Response: 2330397
Conc: 18.37 ug/ml

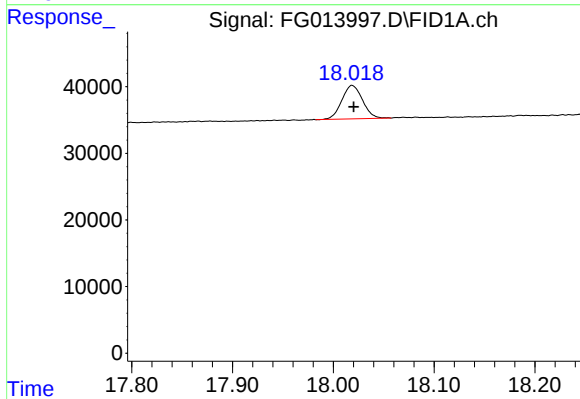

#13 N-TRIACONTANE


R.T.: 18.019 min
Delta R.T.: -0.002 min
Response: 71502
Conc: 0.57 ug/ml

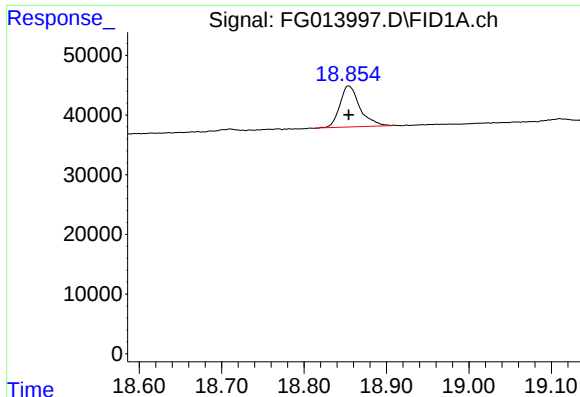

#14 N-DOTRIACONTANE


R.T.: 18.854 min
Delta R.T.: 0.000 min
Response: 115641
Conc: 0.95 ug/ml

Instrument :
FID_G
ClientSampleId :

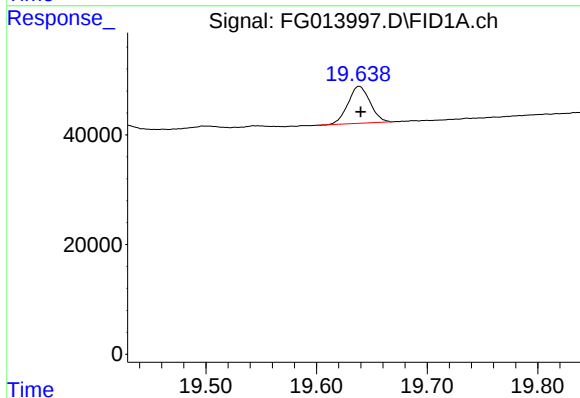


#15 N-TETRATRIACONTANE

R.T.: 19.639 min
Delta R.T.: -0.001 min
Response: 93719
Conc: 0.93 ug/ml

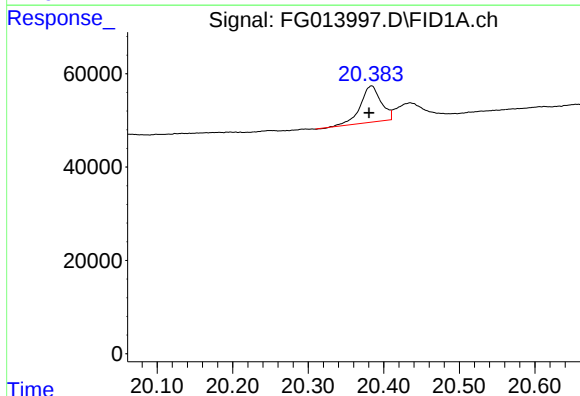


#16 N-HEXATRIACONTANE

R.T.: 20.384 min
Delta R.T.: 0.003 min
Response: 148547
Conc: 1.78 ug/ml

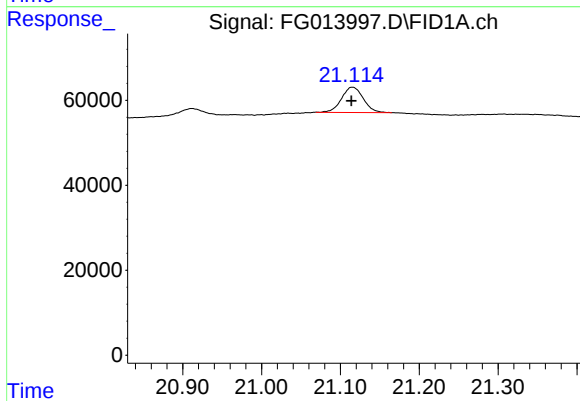

#17 N-OCTATRIACONTANE

R.T.: 21.115 min
Delta R.T.: 0.000 min
Response: 114536
Conc: 1.54 ug/ml

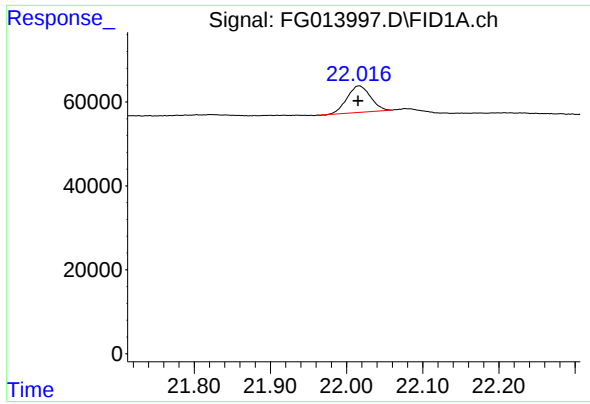

#18 N-TETRACONTANE

R.T.: 22.016 min
Delta R.T.: 0.001 min
Response: 135315
Conc: 1.95 ug/ml

Instrument :
FID_G
ClientSampleId :