

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG073124\
 Data File : FG014007.D
 Signal(s) : FID1A.ch
 Acq On : 31 Jul 2024 21:15
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Aug 01 03:04:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
 Quant Title :
 QLast Update : Tue Jul 23 14:43:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.952	6082068	50.279 ug/ml
Target Compounds			
2) N-DECANE	4.470	6683207	53.605 ug/ml
3) N-DODECANE	6.645	6802140	51.552 ug/ml
4) N-TETRADECANE	8.477	6634452	50.742 ug/ml
5) N-HEXADECANE	10.088	6762240	50.737 ug/ml
6) N-OCTADECANE	11.536	6867540	50.254 ug/ml
7) N-EICOSANE	12.850	6740633	50.434 ug/ml
8) N-DOCOSANE	14.051	6589063	50.055 ug/ml
10) N-TETRACOSANE	15.157	6547226	50.158 ug/ml
11) N-HEXACOSANE	16.180	6472548	50.392 ug/ml
12) N-OCTACOSANE	17.133	6480864	51.097 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG073124\
Data File : FG014007.D
Signal(s) : FID1A.ch
Acq On : 31 Jul 2024 21:15
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Aug 01 03:04:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG072324.M
Quant Title :
QLast Update : Tue Jul 23 14:43:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

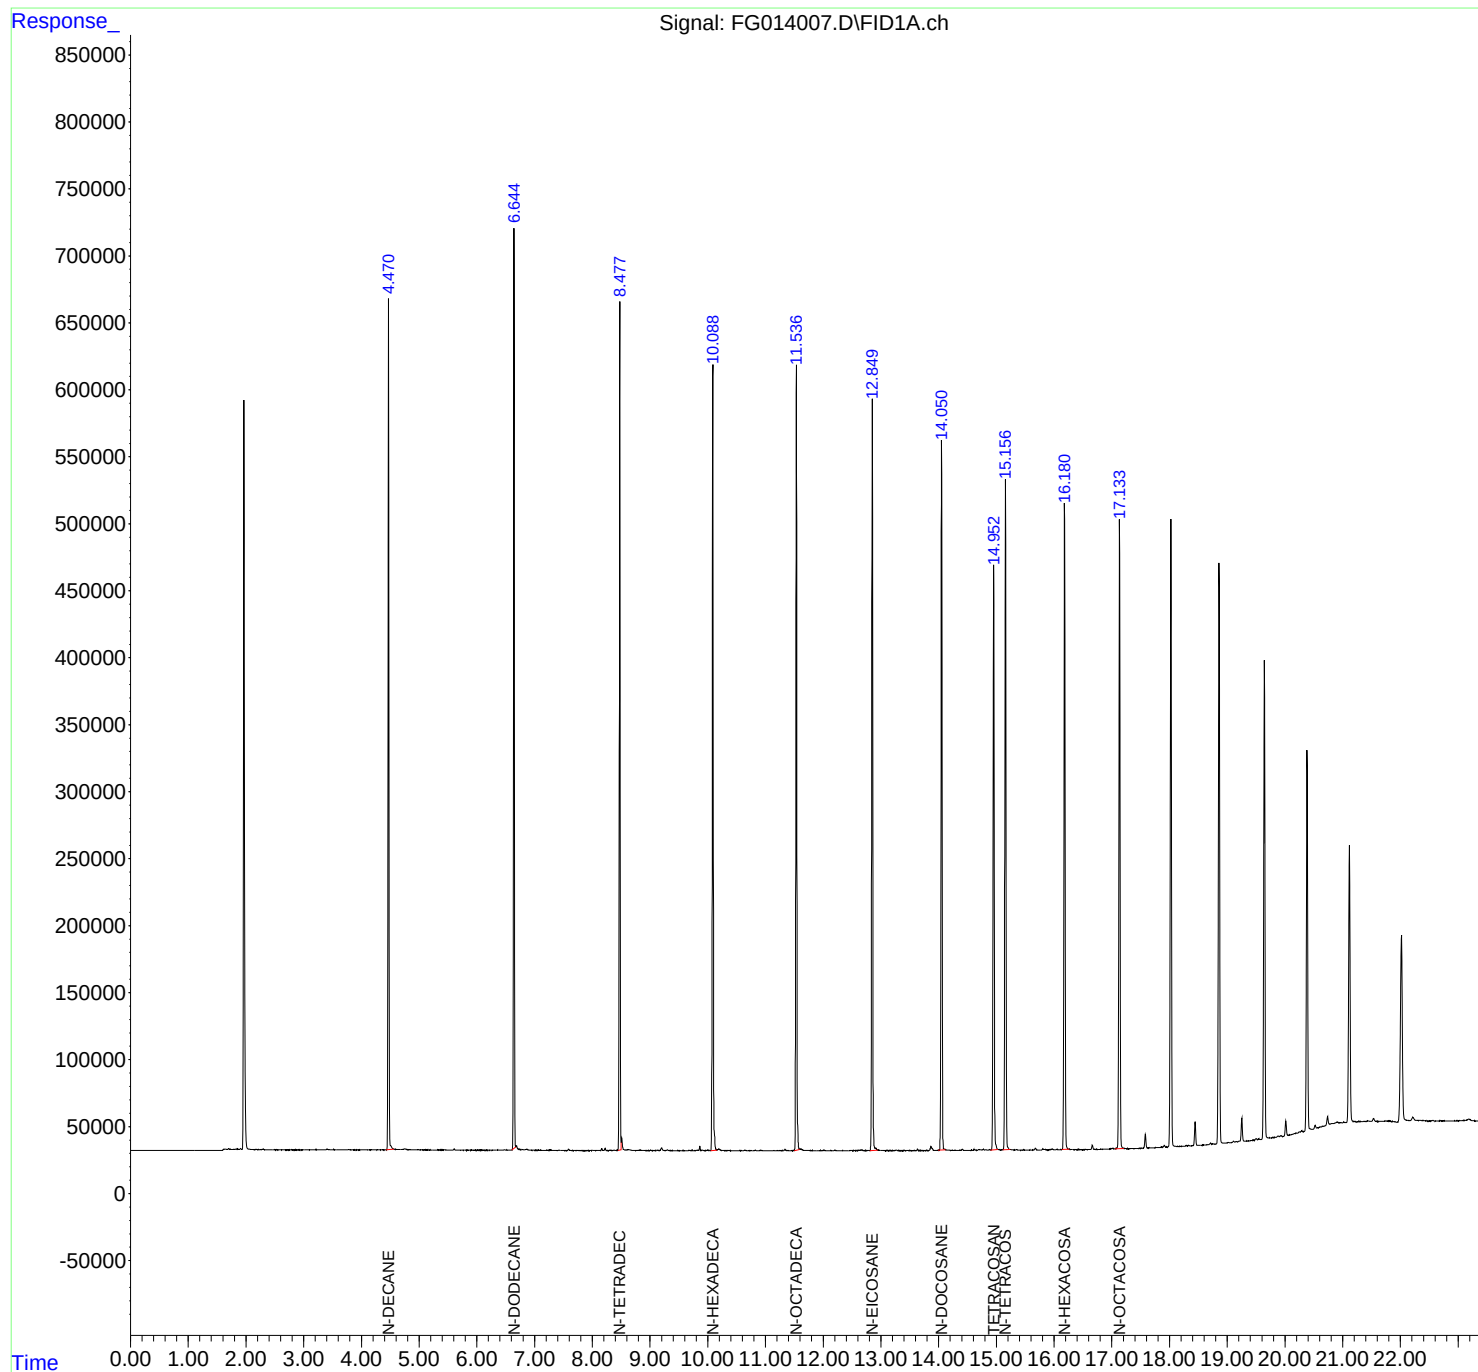


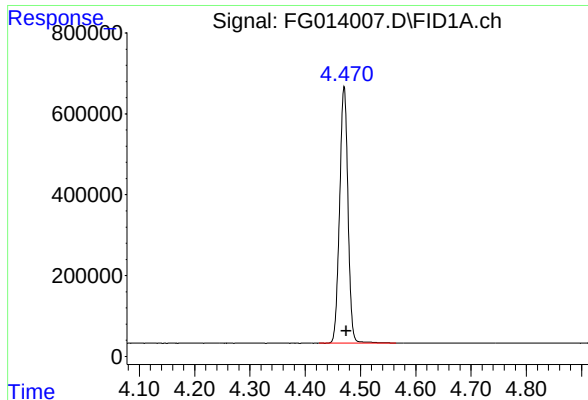

#2 N-DECANE


R.T.: 4.470 min
Delta R.T.: -0.004 min
Response: 6683207
Conc: 53.60 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

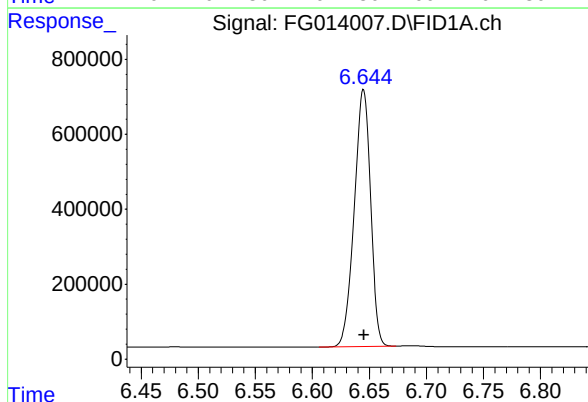


#3 N-DODECANE

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 6802140
Conc: 51.55 ug/ml

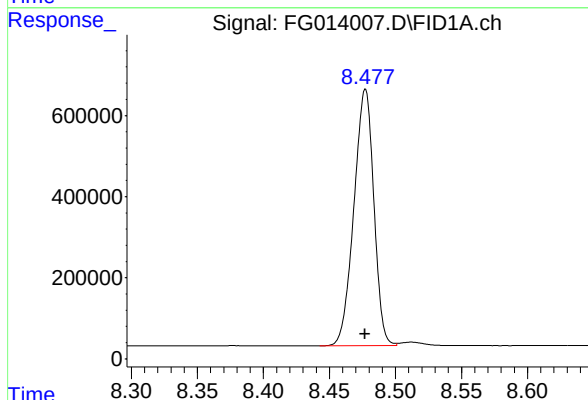


#4 N-TETRADECANE

R.T.: 8.477 min
Delta R.T.: 0.000 min
Response: 6634452
Conc: 50.74 ug/ml

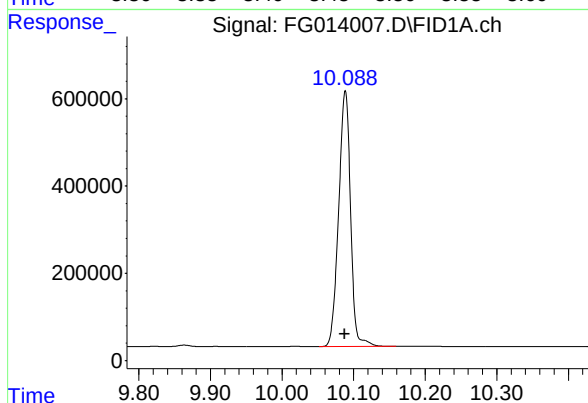

#5 N-HEXADECANE


R.T.: 10.088 min
Delta R.T.: 0.000 min
Response: 6762240
Conc: 50.74 ug/ml

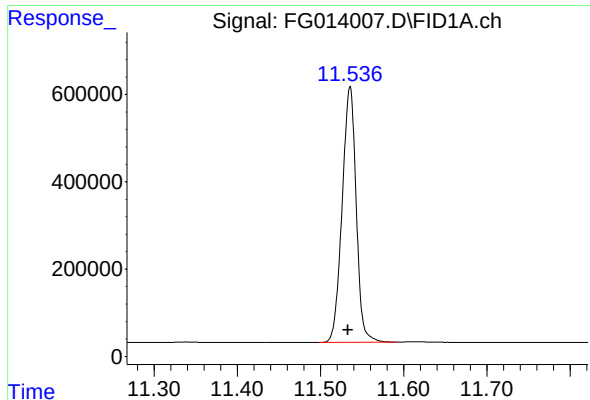

#6 N-OCTADECANE


R.T.: 11.536 min
Delta R.T.: 0.003 min
Response: 6867540
Conc: 50.25 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

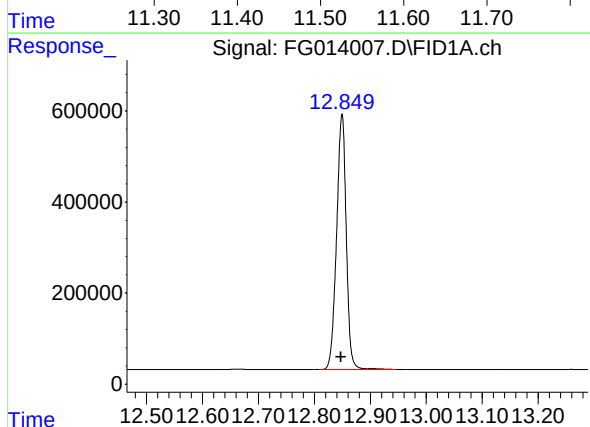


#7 N-EICOSANE

R.T.: 12.850 min
Delta R.T.: 0.002 min
Response: 6740633
Conc: 50.43 ug/ml

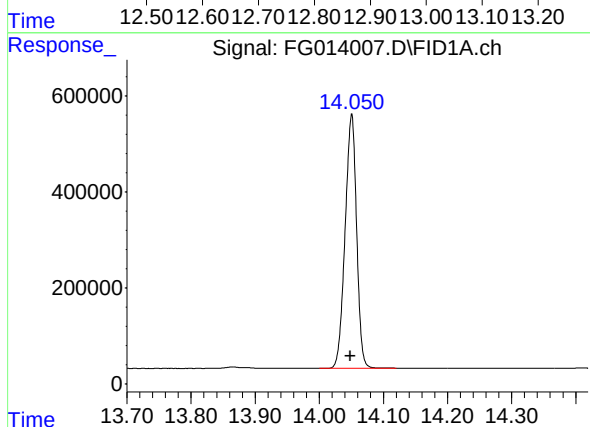


#8 N-DOCOSANE

R.T.: 14.051 min
Delta R.T.: 0.002 min
Response: 6589063
Conc: 50.05 ug/ml

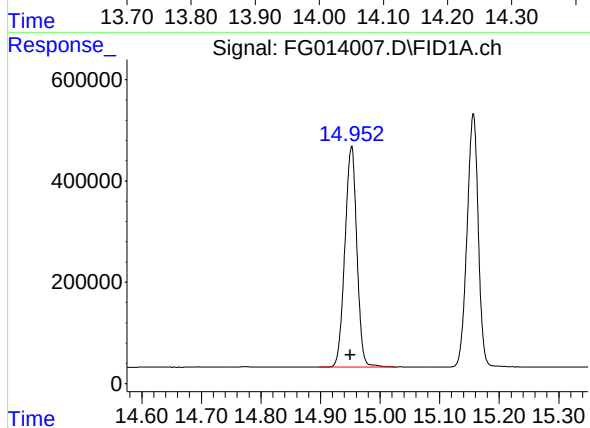

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.952 min
Delta R.T.: 0.002 min
Response: 6082068
Conc: 50.28 ug/ml

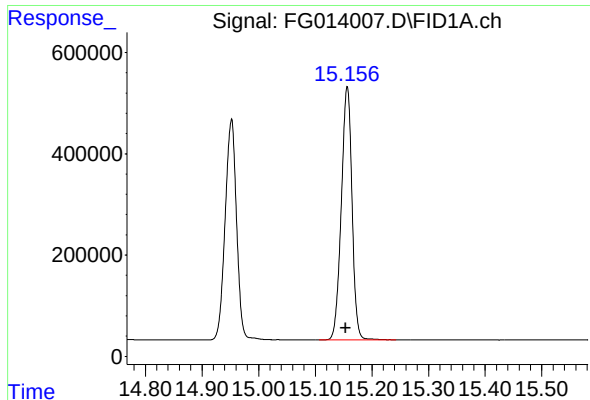

#10 N-TETRACOSANE


R.T.: 15.157 min
Delta R.T.: 0.003 min
Response: 6547226
Conc: 50.16 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

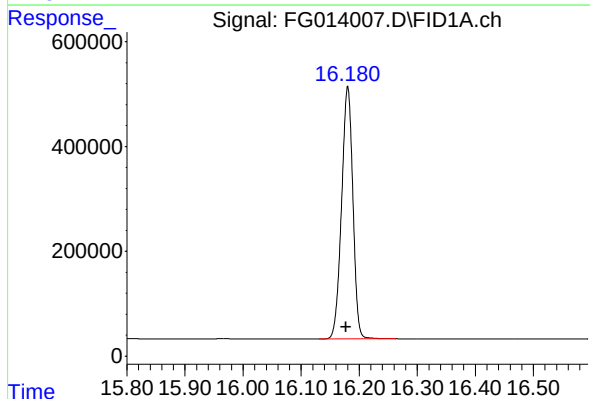

#11 N-HEXACOSANE

R.T.: 16.180 min
Delta R.T.: 0.003 min
Response: 6472548
Conc: 50.39 ug/ml

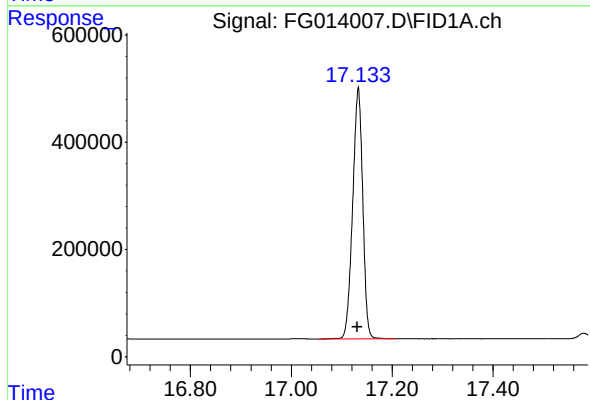

#12 N-OCTACOSANE

R.T.: 17.133 min
Delta R.T.: 0.003 min
Response: 6480864
Conc: 51.10 ug/ml